

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031020\
 Data File : FG006802.D
 Signal(s) : FID1A.ch
 Acq On : 11 Mar 2020 02:34
 Operator : DD\AJ
 Sample : L1852-22 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 11 07:15:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030920.M
 Quant Title :
 QLast Update : Tue Mar 10 08:10:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.700	124609	1.484 ug/ml
Target Compounds			
2) N-DECANE	4.816	108872	1.305 ug/ml
11) N-HEXACOSANE	15.886	92795	0.986 ug/ml
12) N-OCTACOSANE	16.806	85423	0.910 ug/ml
13) N-TRIACONTANE	17.665	201488	2.147 ug/ml
14) N-DOTRIACONTANE	18.468	181391	2.081 ug/ml
15) N-TETRATRIACONTANE	19.223	170594	2.308 ug/ml
16) N-HEXATRIACONTANE	19.937	788352	13.180 ug/ml
17) N-OCTATRIACONTANE	20.631	72751	1.542 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031020\
Data File : FG006802.D
Signal(s) : FID1A.ch
Acq On : 11 Mar 2020 02:34
Operator : DD\AJ
Sample : L1852-22 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 11 07:15:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030920.M
Quant Title :
QLast Update : Tue Mar 10 08:10:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

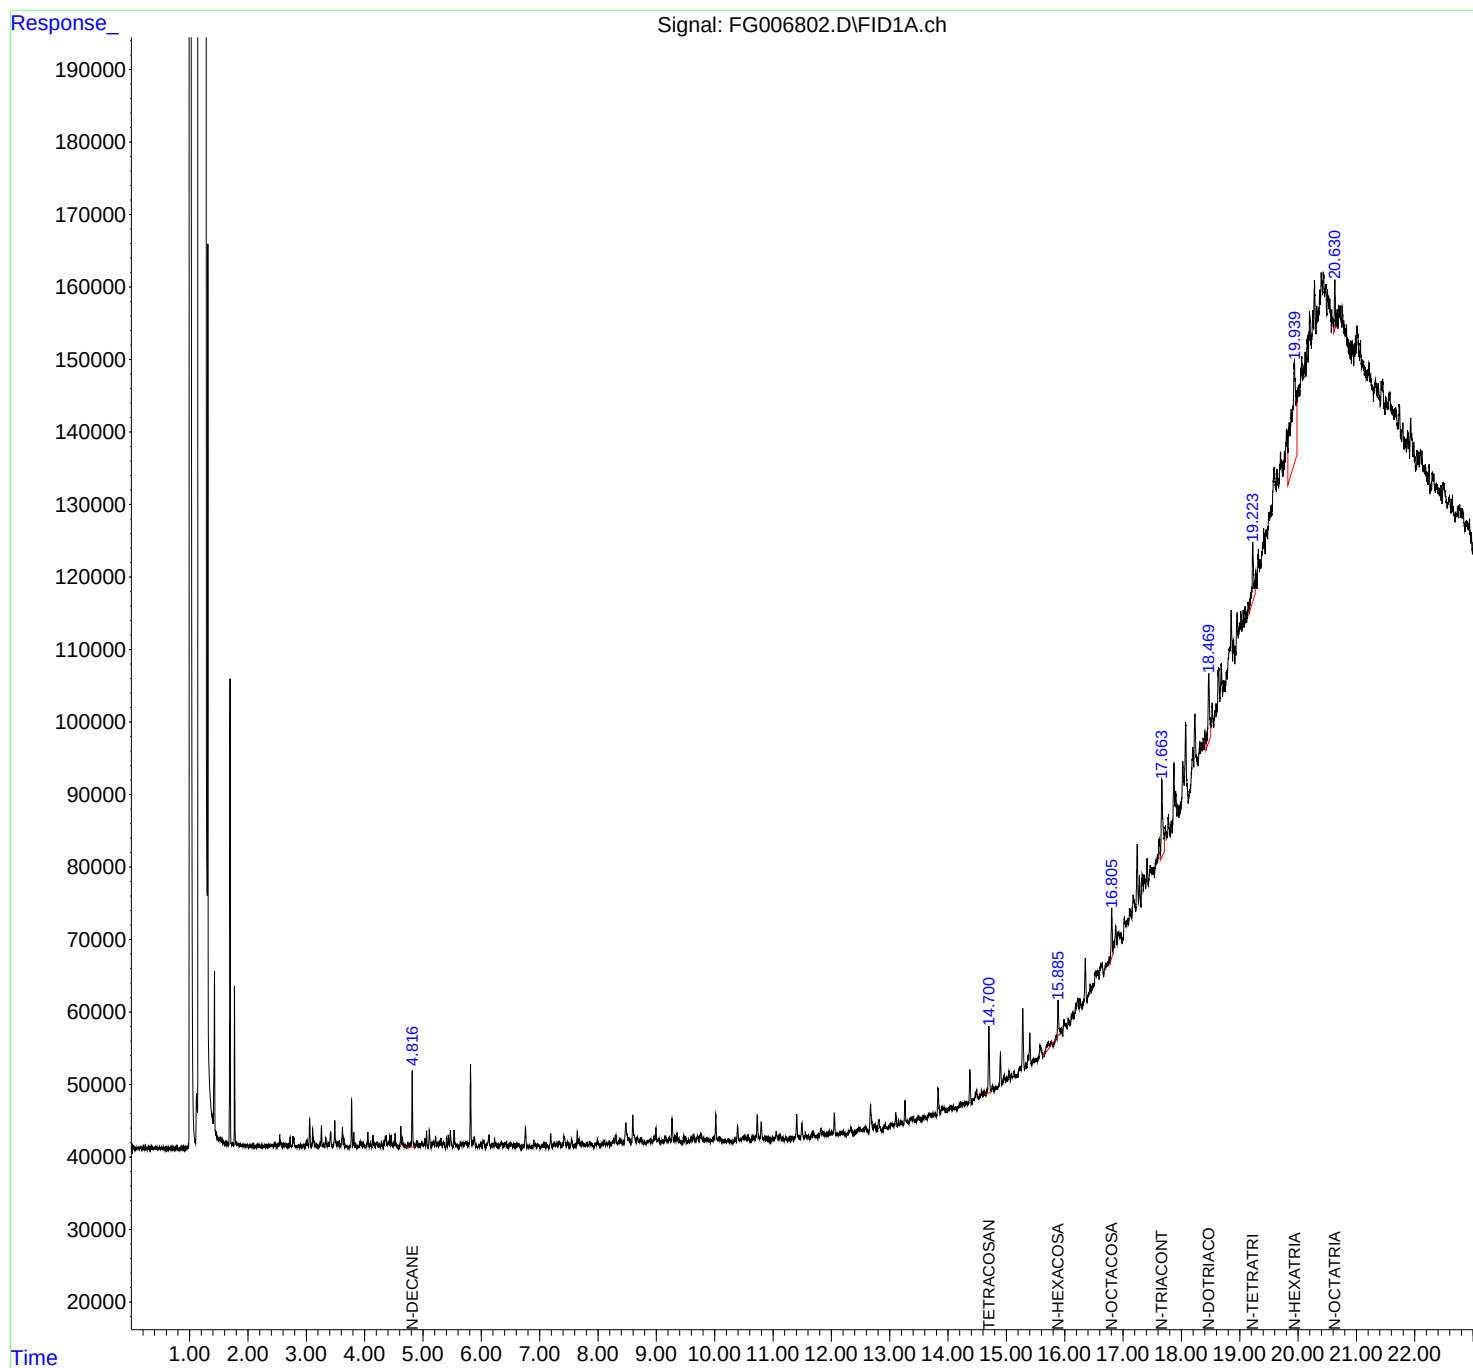


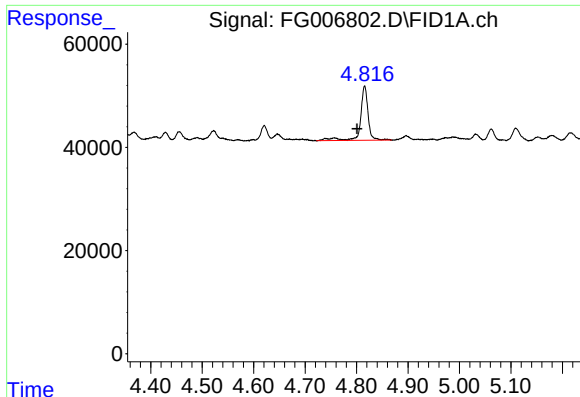

#2 N-DECANE


R.T.: 4.816 min
Delta R.T.: 0.015 min
Response: 108872
Conc: 1.31 ug/ml

Instrument :
FID_G
ClientSampleId :

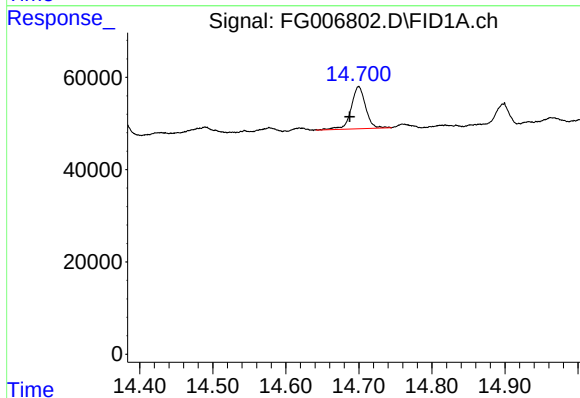


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.700 min
Delta R.T.: 0.012 min
Response: 124609
Conc: 1.48 ug/ml

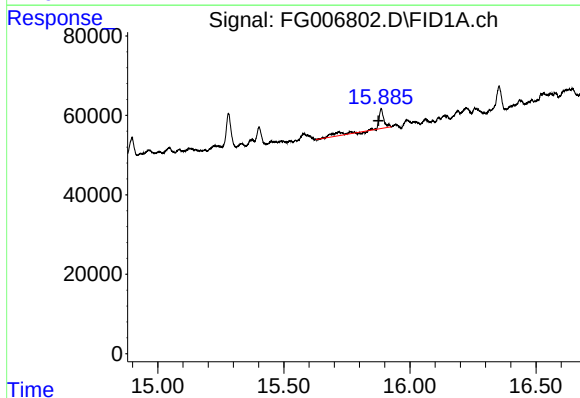


#11 N-HEXACOSANE

R.T.: 15.886 min
Delta R.T.: 0.011 min
Response: 92795
Conc: 0.99 ug/ml

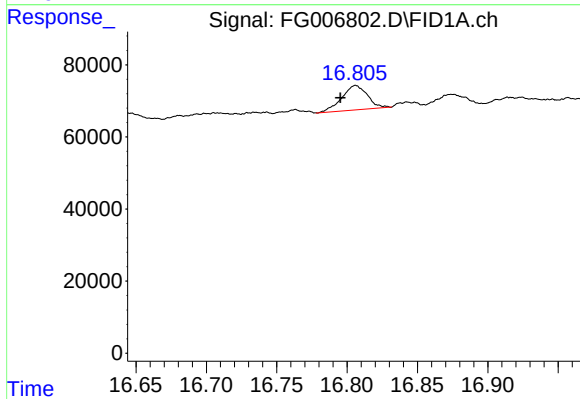

#12 N-OCTACOSANE


R.T.: 16.806 min
Delta R.T.: 0.011 min
Response: 85423
Conc: 0.91 ug/ml

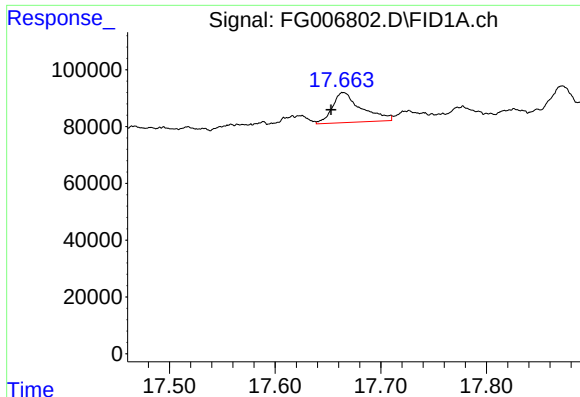

#13 N-TRIACONTANE


R.T.: 17.665 min
Delta R.T.: 0.012 min
Response: 201488
Conc: 2.15 ug/ml

Instrument :
FID_G
ClientSampleId :

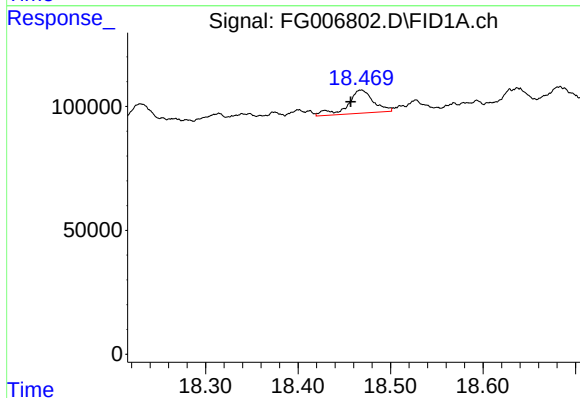


#14 N-DOTRIACONTANE

R.T.: 18.468 min
Delta R.T.: 0.011 min
Response: 181391
Conc: 2.08 ug/ml

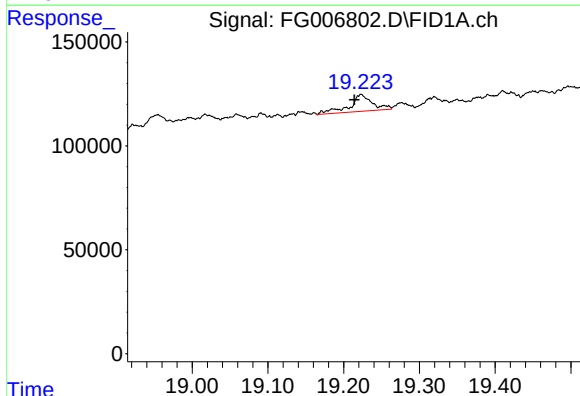


#15 N-TETRATRIACONTANE

R.T.: 19.223 min
Delta R.T.: 0.009 min
Response: 170594
Conc: 2.31 ug/ml

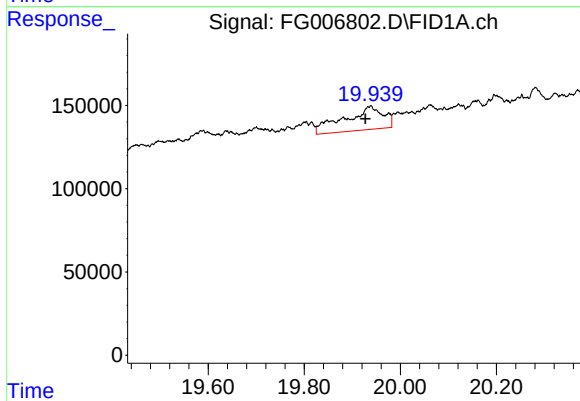

#16 N-HEXATRIACONTANE

R.T.: 19.937 min
Delta R.T.: 0.010 min
Response: 788352
Conc: 13.18 ug/ml

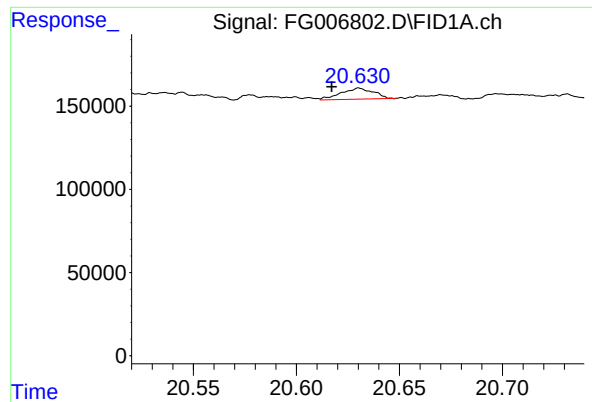

#17 N-OCTATRIACONTANE

R.T.: 20.631 min
Delta R.T.: 0.014 min
Response: 72751
Conc: 1.54 ug/ml

Instrument :
FID_G
ClientSampleId :