

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031020\
 Data File : FG006803.D
 Signal(s) : FID1A.ch
 Acq On : 11 Mar 2020 03:04
 Operator : DD\AJ
 Sample : L1852-22 50X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 11 07:15:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030920.M
 Quant Title :
 QLast Update : Tue Mar 10 08:10:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
13) N-TRIACONTANE	17.665	160293	1.708 ug/ml
14) N-DOTRIACONTANE	18.468	90410	1.037 ug/ml
15) N-TETRATRIACONTANE	19.222	119086	1.611 ug/ml
16) N-HEXATRIACONTANE	19.933	262490	4.388 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031020\
Data File : FG006803.D
Signal(s) : FID1A.ch
Acq On : 11 Mar 2020 03:04
Operator : DD\AJ
Sample : L1852-22 50X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 11 07:15:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030920.M
Quant Title :
QLast Update : Tue Mar 10 08:10:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

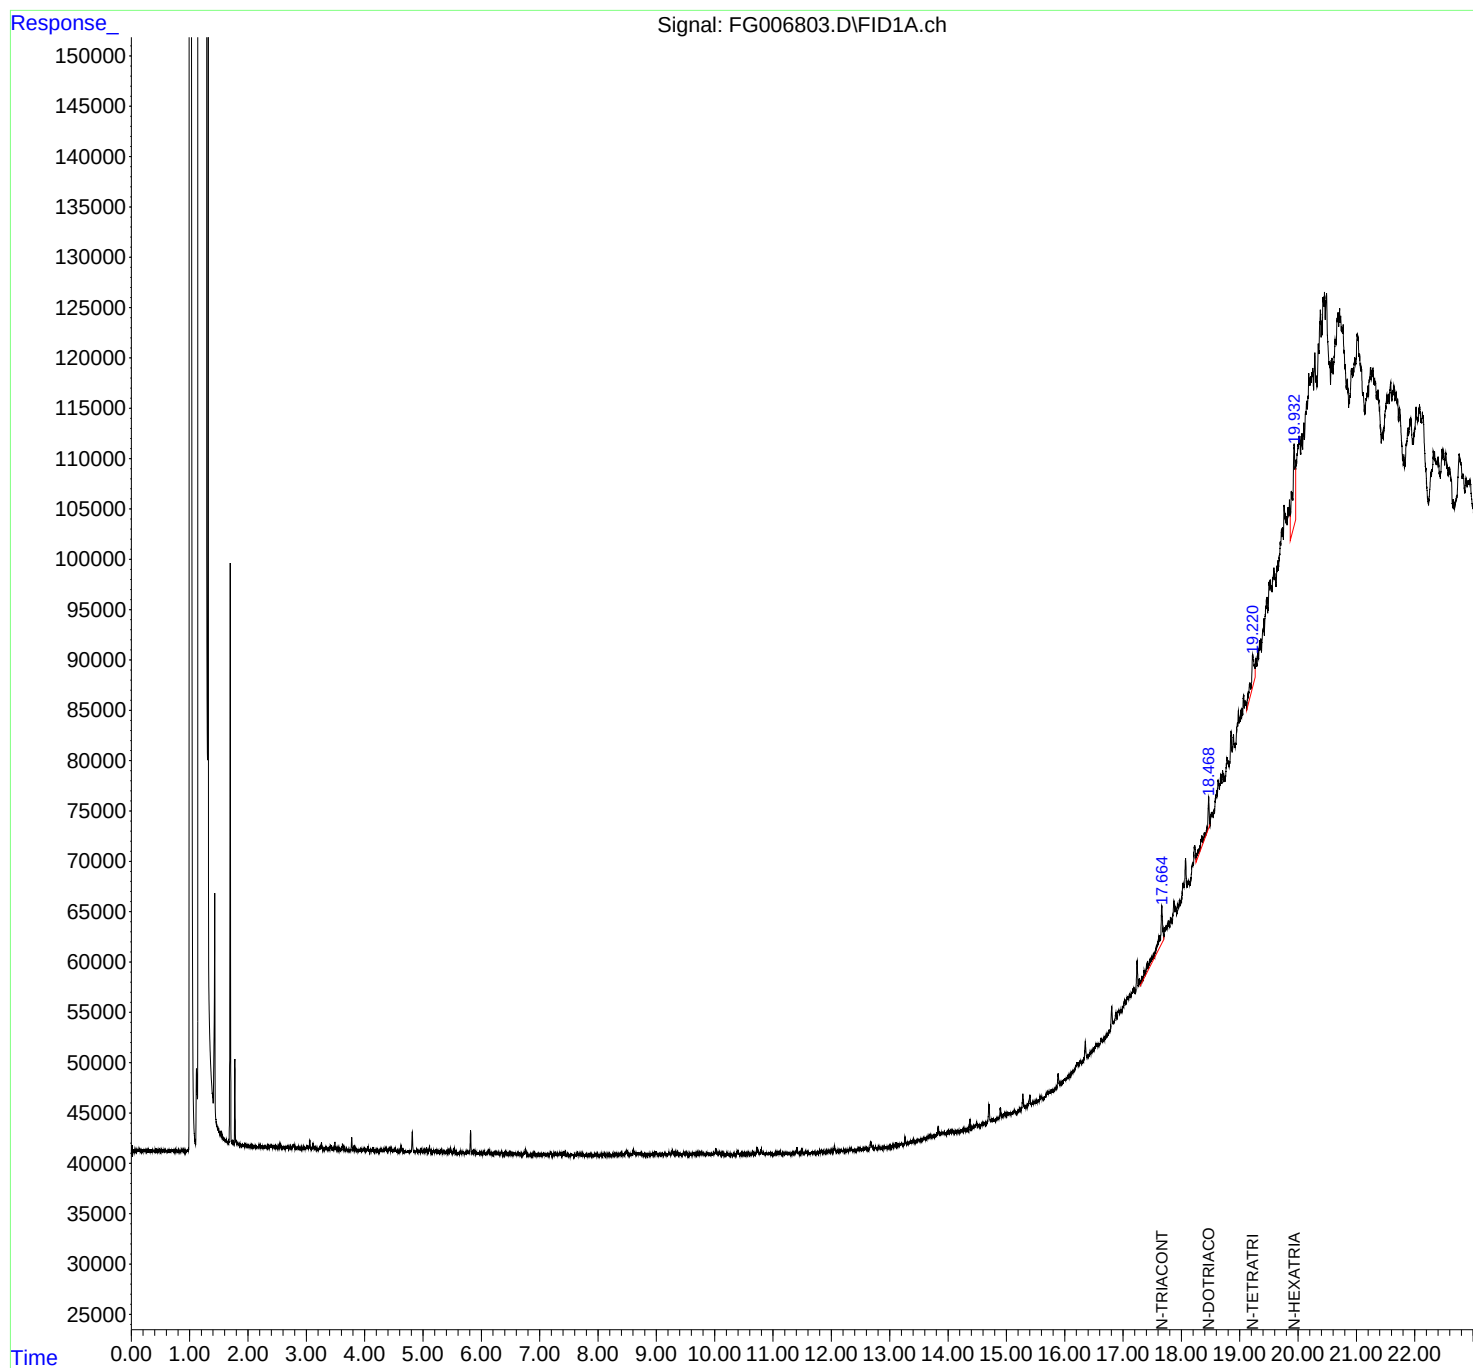


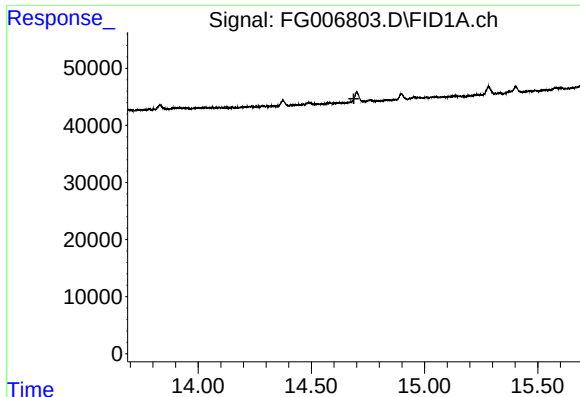

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.688 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

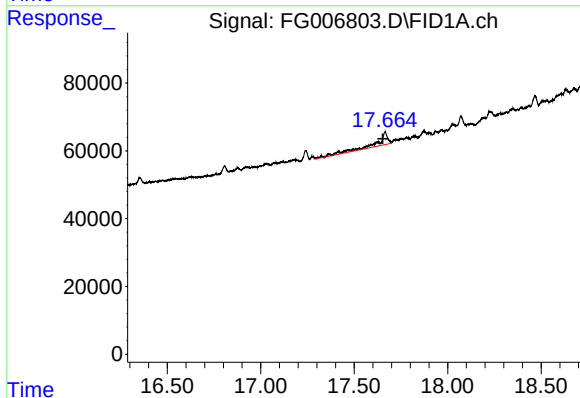


#13 N-TRIACONTANE

R.T.: 17.665 min
Delta R.T.: 0.012 min
Response: 160293
Conc: 1.71 ug/ml

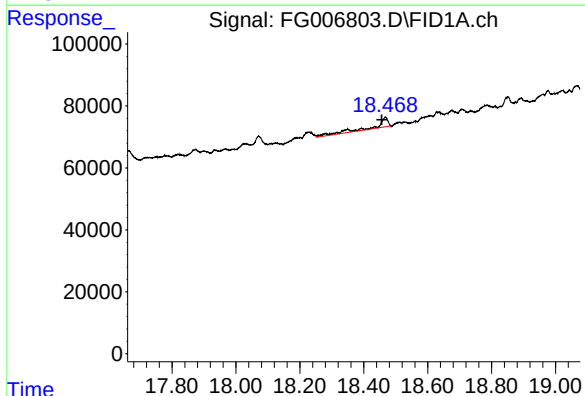


#14 N-DOTRIACONTANE

R.T.: 18.468 min
Delta R.T.: 0.011 min
Response: 90410
Conc: 1.04 ug/ml

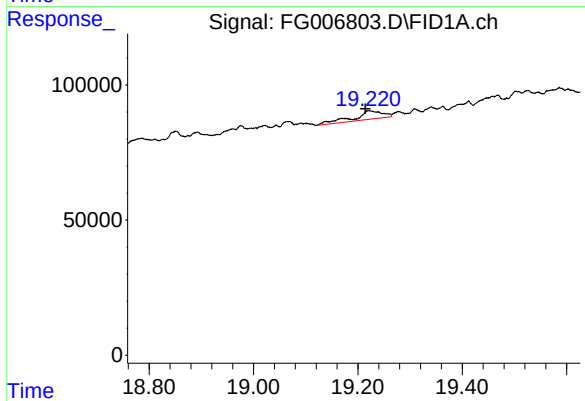

#15 N-TETRATRIACONTANE

R.T.: 19.222 min
Delta R.T.: 0.007 min
Response: 119086
Conc: 1.61 ug/ml

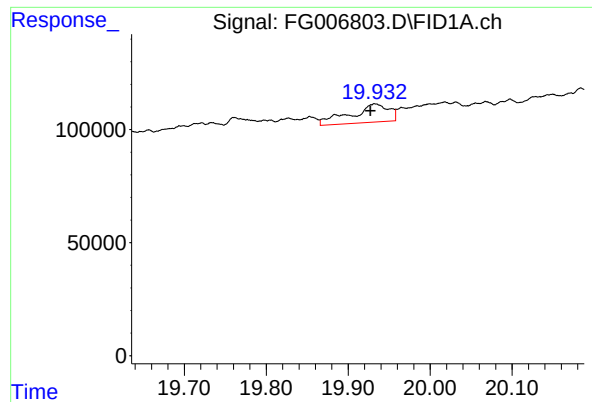

#16 N-HEXATRIACONTANE

R.T.: 19.933 min
Delta R.T.: 0.005 min
Response: 262490
Conc: 4.39 ug/ml

Instrument :
FID_G
ClientSampleId :