

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031021\
Data File : FG007676.D
Signal(s) : FID1A.ch
Acq On : 10 Mar 2021 12:03
Operator : DD\AJ
Sample : M1597-01 20X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 10 23:52:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030421.M
Quant Title :
QLast Update : Fri Mar 05 08:57:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.363	105514	0.823 ug/ml
15)	N-TETRATRIACONTANE	19.151	25082	0.209 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031021\
Data File : FG007676.D
Signal(s) : FID1A.ch
Acq On : 10 Mar 2021 12:03
Operator : DD\AJ
Sample : M1597-01 20X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 10 23:52:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030421.M
Quant Title :
QLast Update : Fri Mar 05 08:57:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

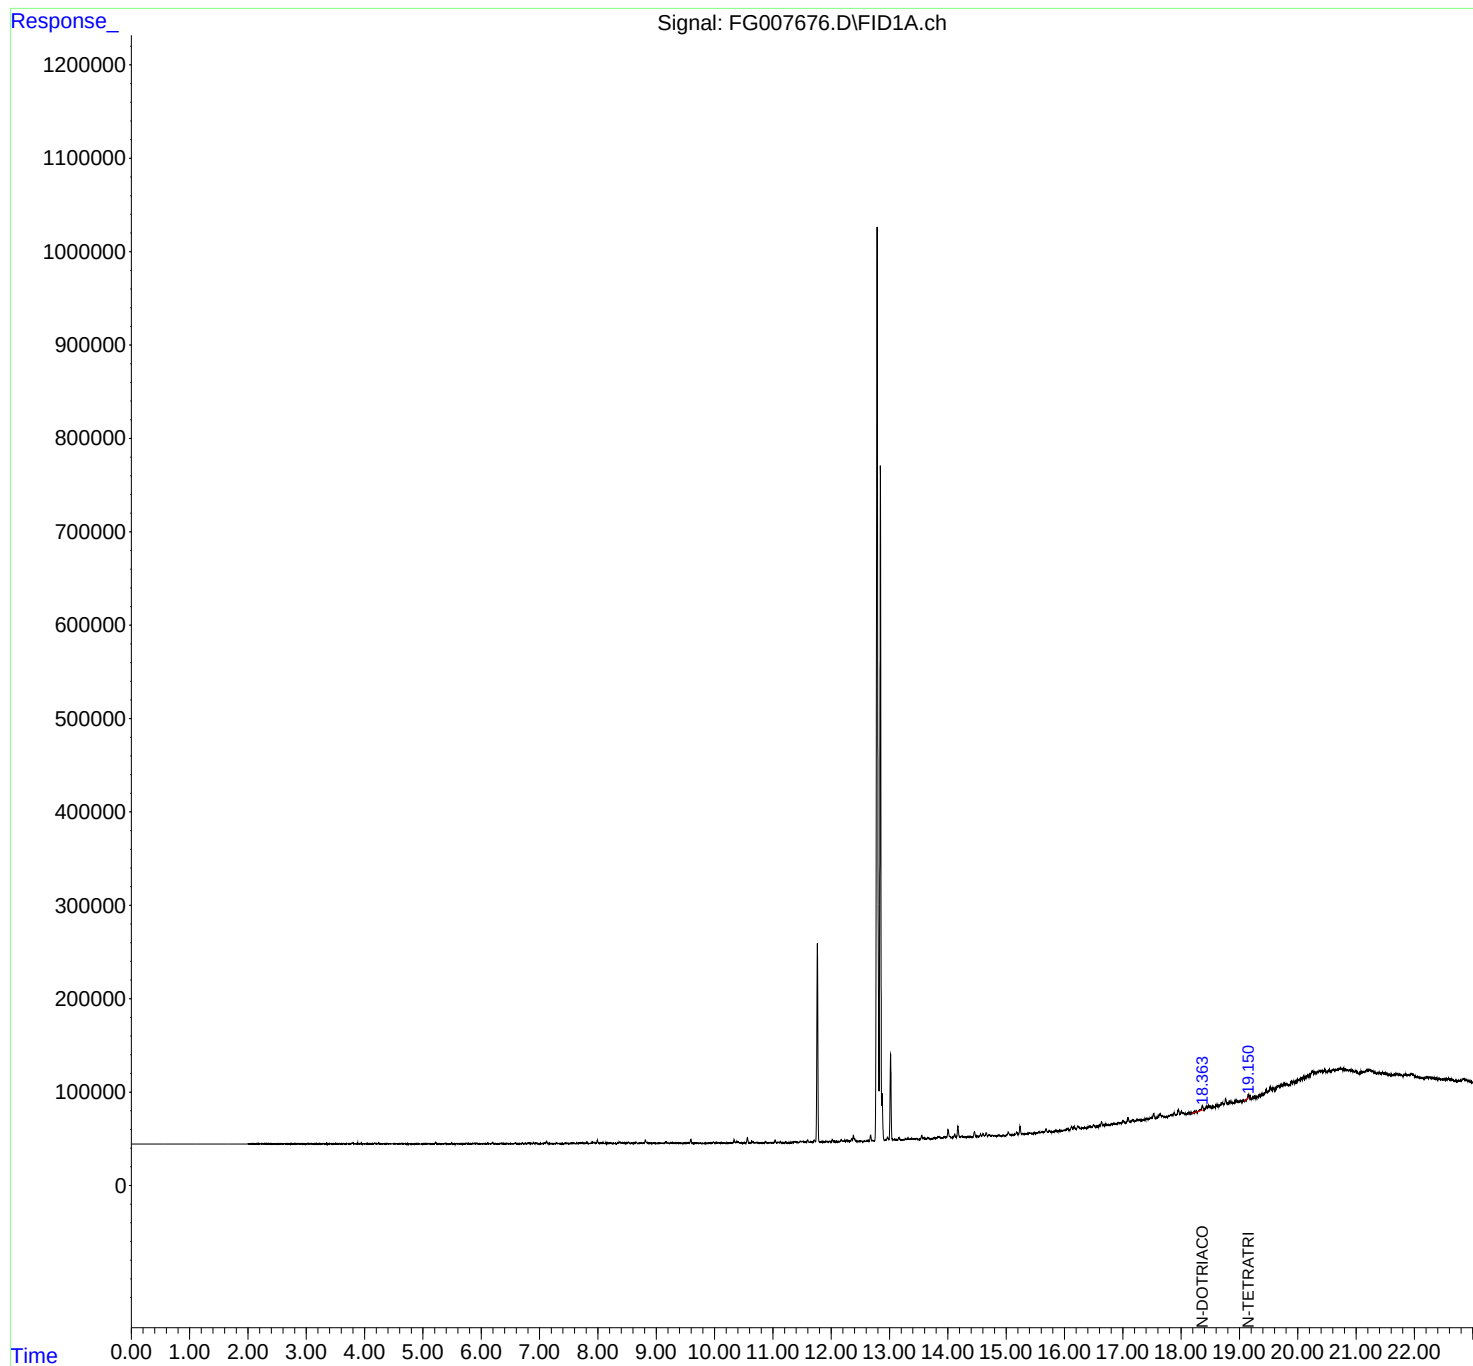


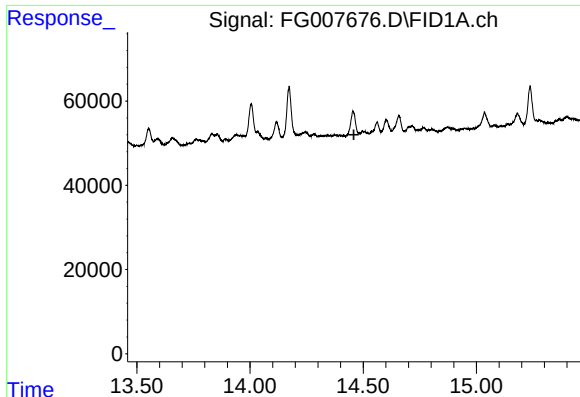

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.459 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

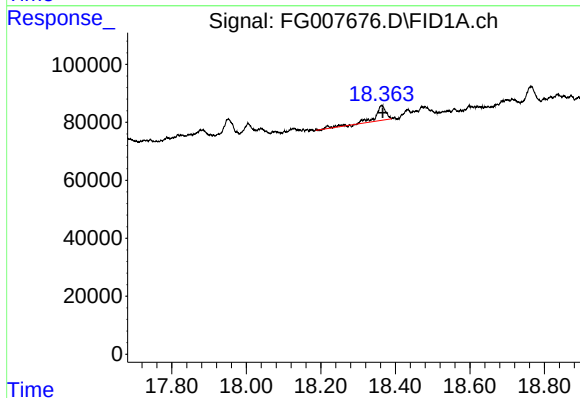

#14 N-DOTRIACONTANE

R.T.: 18.363 min
Delta R.T.: -0.003 min
Response: 105514
Conc: 0.82 ug/ml

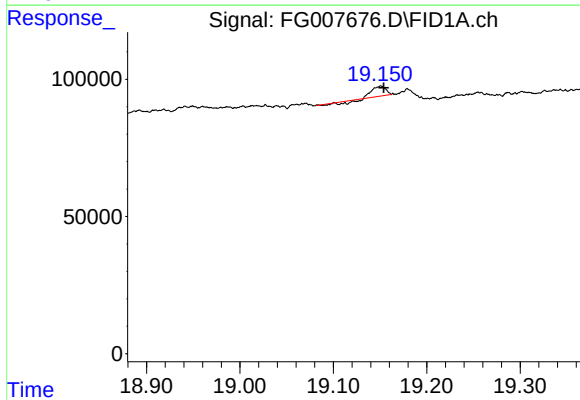

#15 N-TETRATRIACONTANE

R.T.: 19.151 min
Delta R.T.: -0.003 min
Response: 25082
Conc: 0.21 ug/ml