

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031021\
 Data File : FG007676.D
 Signal(s) : FID1A.ch
 Acq On : 10 Mar 2021 12:03
 Operator : DD\AJ
 Sample : M1597-01 20X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 AU-06-030821

Manual Integrations
 APPROVED

Ankita
 3/11/2021 9:20:57 AM

Integration File: autoint1.e
 Quant Time: Mar 10 23:52:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030421.M
 Quant Title :
 QLast Update : Fri Mar 05 08:57:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.454	98899	0.742 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031021\
Data File : FG007676.D
Signal(s) : FID1A.ch
Acq On : 10 Mar 2021 12:03
Operator : DD\AJ
Sample : M1597-01 20X
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
AU-06-030821


Manual Integrations
APPROVED

Ankita
3/11/2021 9:20:57 AM

Integration File: autoint1.e
Quant Time: Mar 10 23:52:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030421.M
Quant Title :
QLast Update : Fri Mar 05 08:57:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

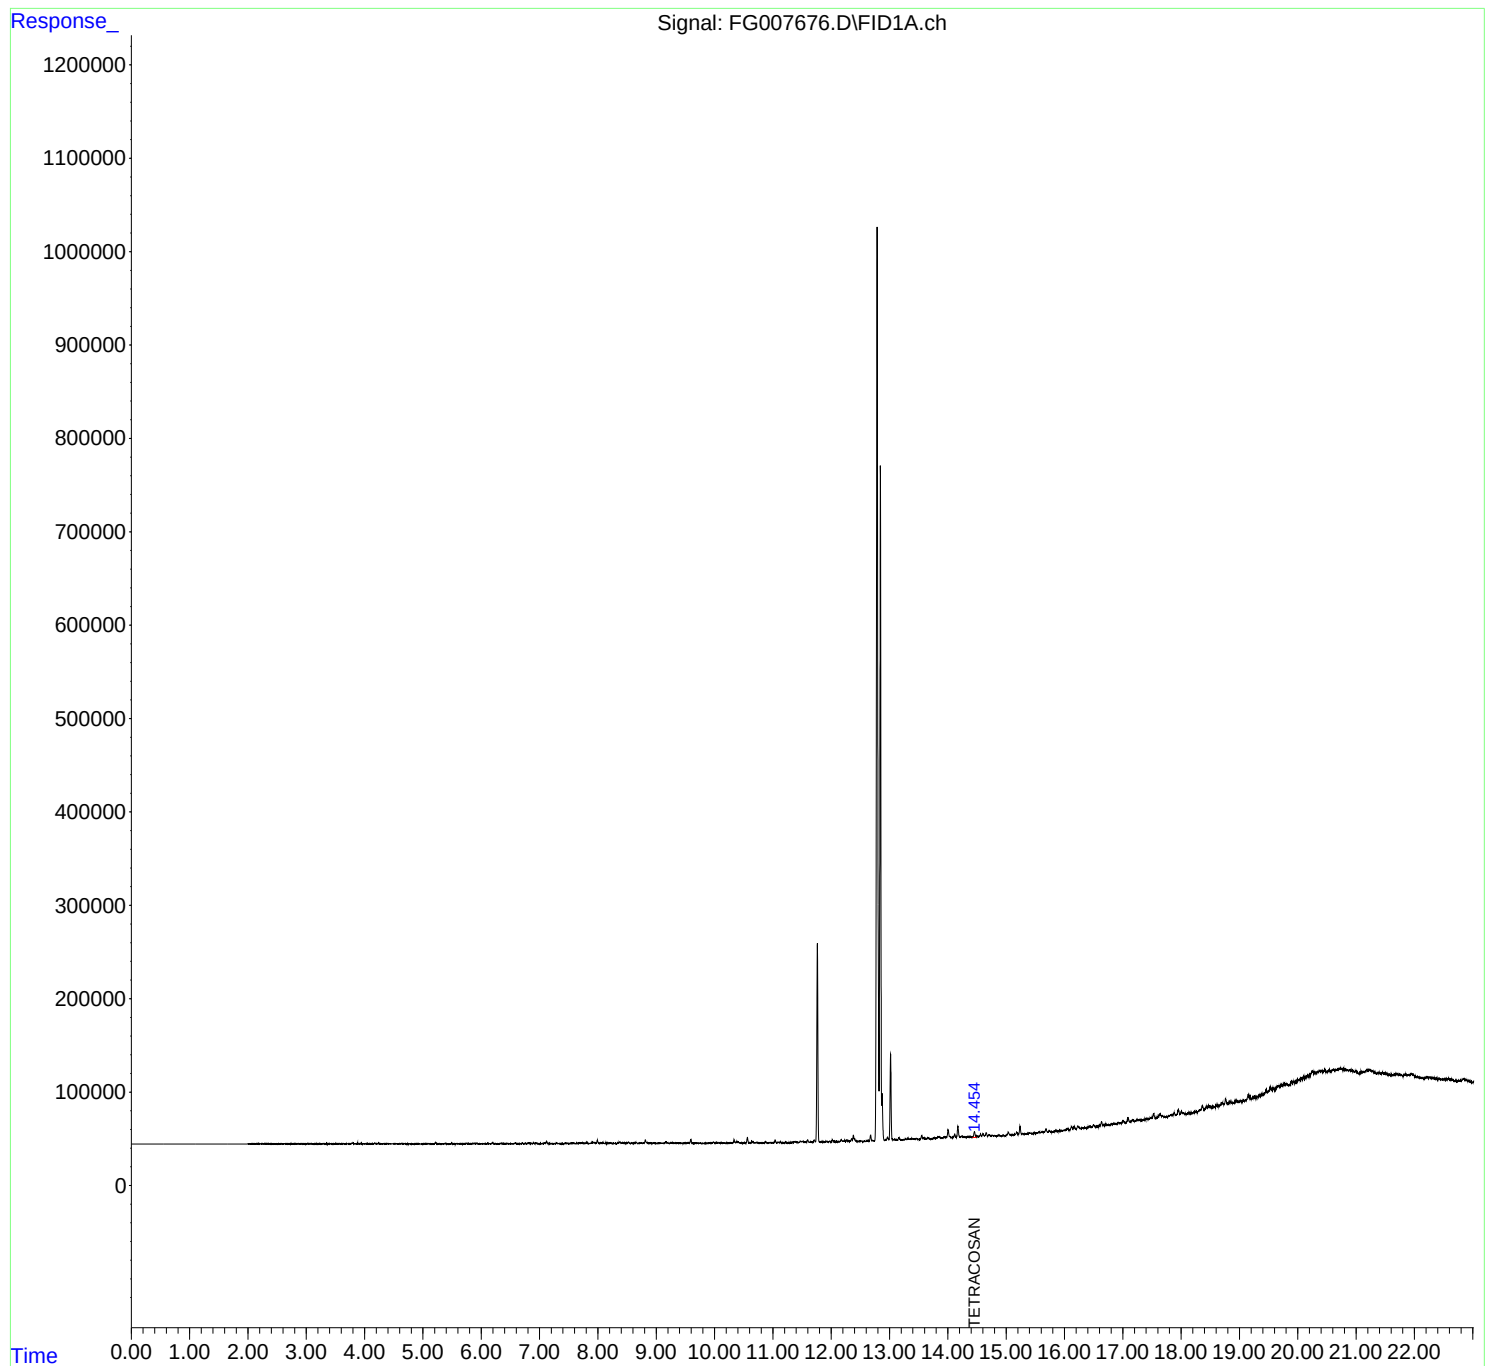

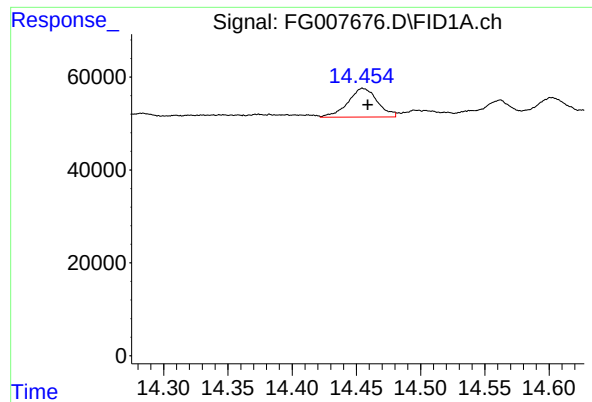

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.454 min
Delta R.T.: -0.004 min
Response: 98899
Conc: 0.74 ug/ml m

Instrument :
FID_G
ClientSampleId :
AU-06-030821

Manual Integrations
APPROVED

Ankita
3/11/2021 9:20:57 AM