

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031120\
 Data File : FG006822.D
 Signal(s) : FID1A.ch
 Acq On : 11 Mar 2020 18:04
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 11 18:20:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030920.M
 Quant Title :
 QLast Update : Tue Mar 10 08:10:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.710	3667771	43.678 ug/ml
Target Compounds			
2) N-DECANE	4.822	4596141	55.109 ug/ml
3) N-DODECANE	6.765	4704453	54.007 ug/ml
4) N-TETRADECANE	8.488	4643766	51.124 ug/ml
5) N-HEXADECANE	10.026	4606850	47.965 ug/ml
6) N-OCTADECANE	11.416	4507438	45.706 ug/ml
7) N-EICOSANE	12.681	4391658	44.479 ug/ml
8) N-DOCOSANE	13.840	4286922	43.873 ug/ml
10) N-TETRACOSANE	14.909	4217240	43.748 ug/ml
11) N-HEXACOSANE	15.897	4152438	44.116 ug/ml
12) N-OCTACOSANE	16.816	4186067	44.572 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031120\
Data File : FG006822.D
Signal(s) : FID1A.ch
Acq On : 11 Mar 2020 18:04
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 11 18:20:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030920.M
Quant Title :
QLast Update : Tue Mar 10 08:10:01 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

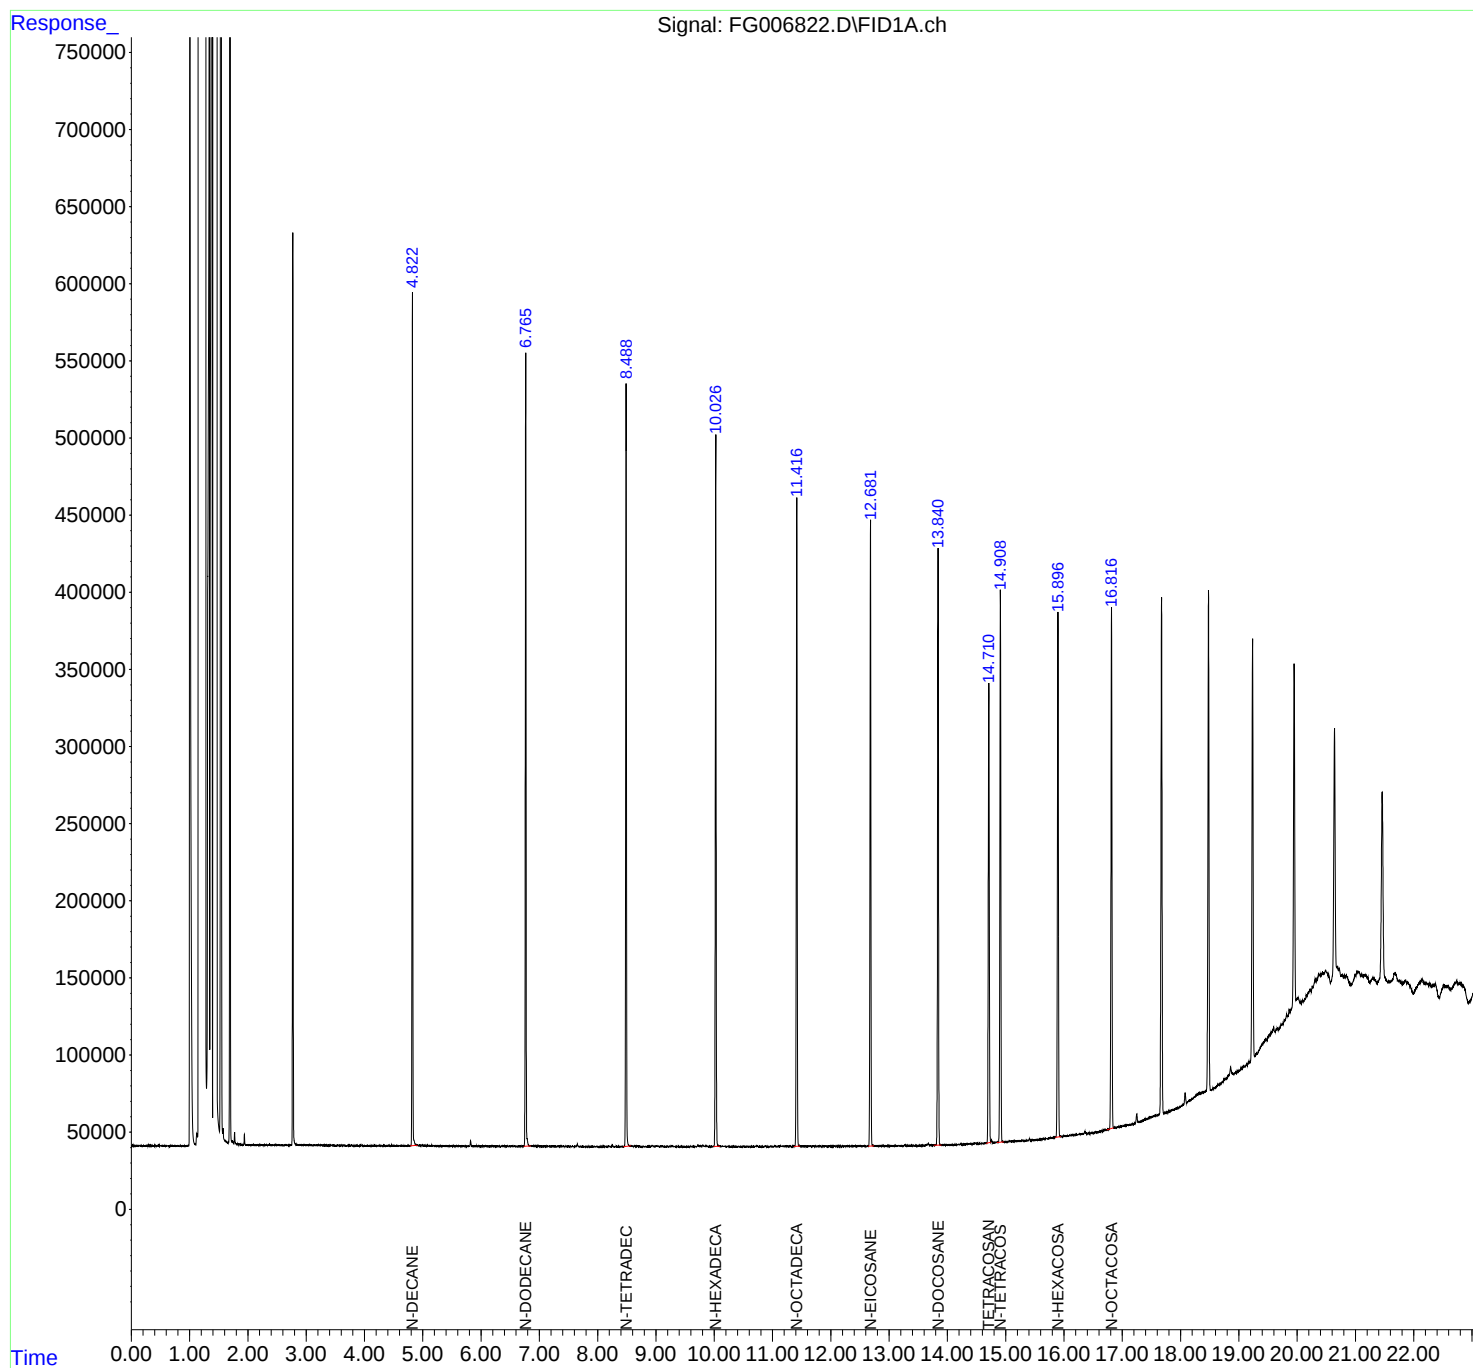

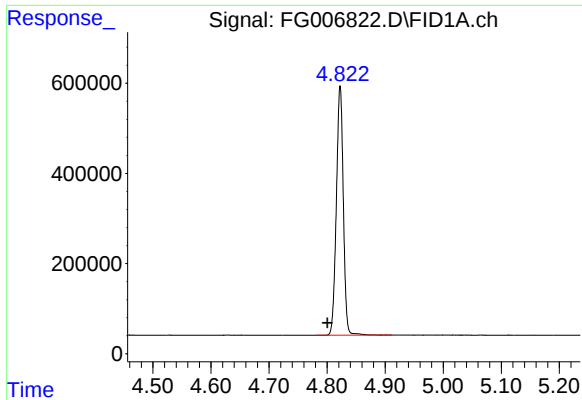


#2 N-DECANE

R.T.: 4.822 min
Delta R.T.: 0.022 min
Response: 4596141
Conc: 55.11 ug/ml

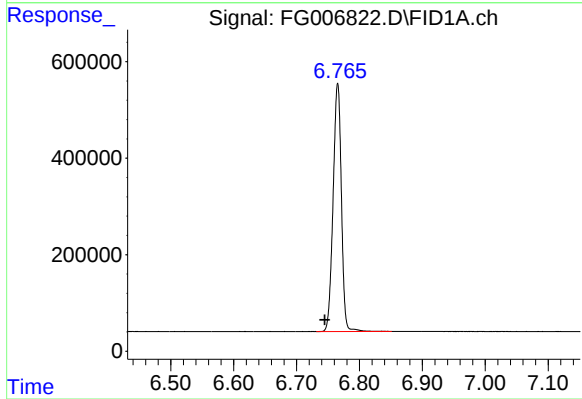


#3 N-DODECANE

R.T.: 6.765 min
Delta R.T.: 0.020 min
Response: 4704453
Conc: 54.01 ug/ml

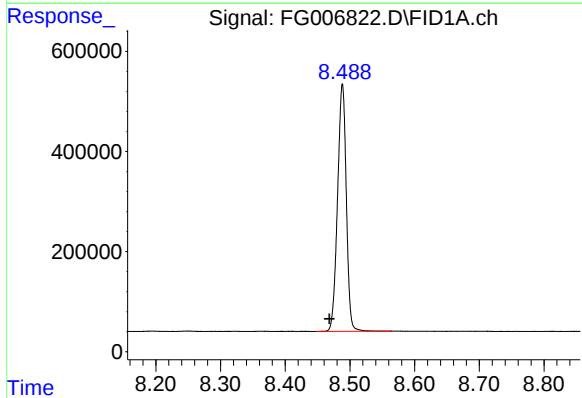


#4 N-TETRADECANE

R.T.: 8.488 min
Delta R.T.: 0.020 min
Response: 4643766
Conc: 51.12 ug/ml

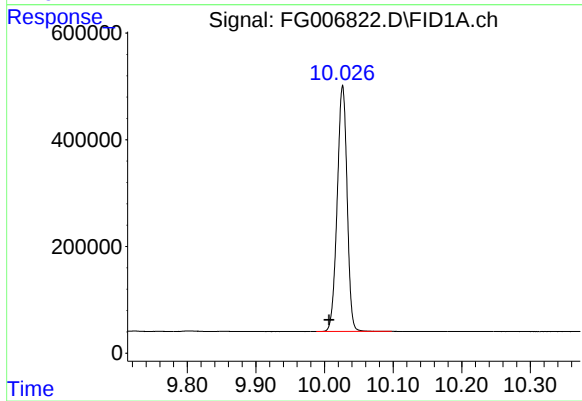


#5 N-HEXADECANE

R.T.: 10.026 min
Delta R.T.: 0.020 min
Response: 4606850
Conc: 47.96 ug/ml

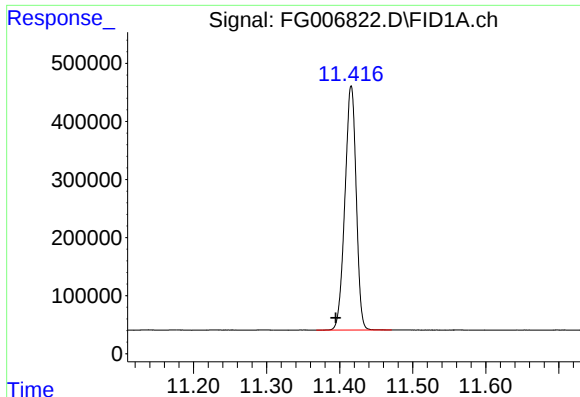


#6 N-OCTADECANE

R.T.: 11.416 min
Delta R.T.: 0.021 min
Response: 4507438
Conc: 45.71 ug/ml

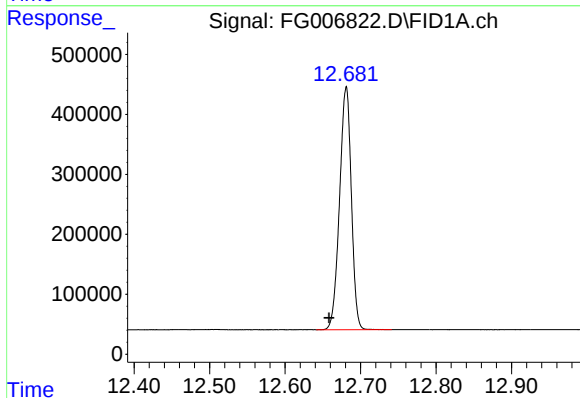


#7 N-EICOSANE

R.T.: 12.681 min
Delta R.T.: 0.022 min
Response: 4391658
Conc: 44.48 ug/ml

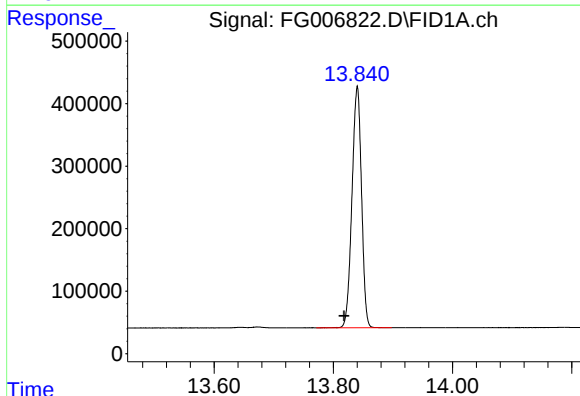


#8 N-DOCOSANE

R.T.: 13.840 min
Delta R.T.: 0.022 min
Response: 4286922
Conc: 43.87 ug/ml

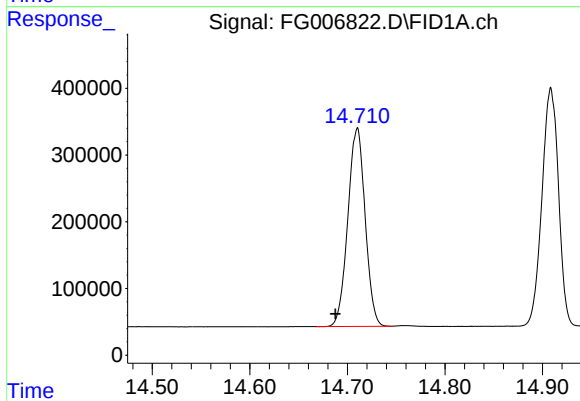


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.710 min
Delta R.T.: 0.022 min
Response: 3667771
Conc: 43.68 ug/ml

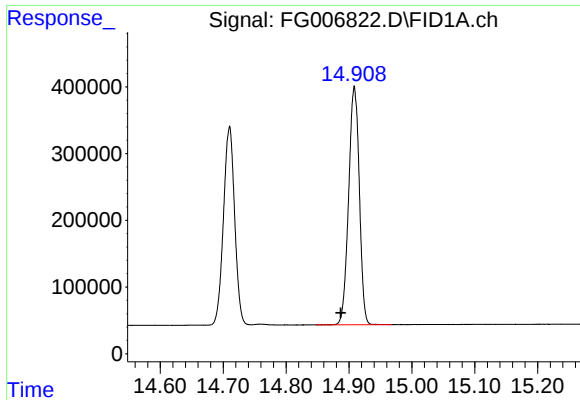


#10 N-TETRACOSANE

R.T.: 14.909 min
Delta R.T.: 0.022 min
Response: 4217240
Conc: 43.75 ug/ml

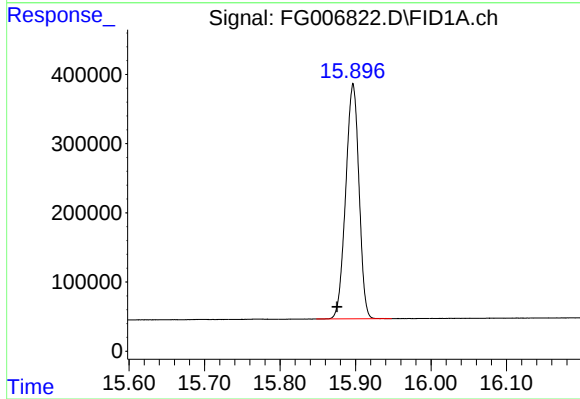

#11 N-HEXACOSANE

R.T.: 15.897 min
Delta R.T.: 0.021 min
Response: 4152438
Conc: 44.12 ug/ml

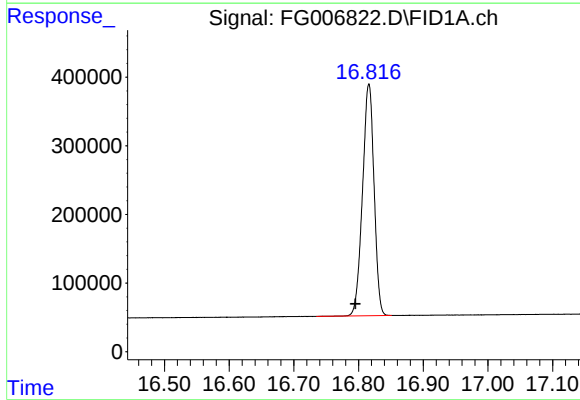

#12 N-OCTACOSANE

R.T.: 16.816 min
Delta R.T.: 0.021 min
Response: 4186067
Conc: 44.57 ug/ml