

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031225\
Data File : FG015470.D
Signal(s) : FID1A.ch
Acq On : 12 Mar 2025 10:00
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 13 03:16:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030325.M
Quant Title :
QLast Update : Mon Mar 03 14:06:11 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
13)	N-TRIACONTANE	18.097	18113	0.156 ug/ml
14)	N-DOTRIACONTANE	18.927	18450	0.160 ug/ml
15)	N-TETRATRIACONTANE	19.717	20433	0.190 ug/ml
16)	N-HEXATRIACONTANE	20.512f	21234	0.221 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031225\
Data File : FG015470.D
Signal(s) : FID1A.ch
Acq On : 12 Mar 2025 10:00
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 13 03:16:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030325.M
Quant Title :
QLast Update : Mon Mar 03 14:06:11 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

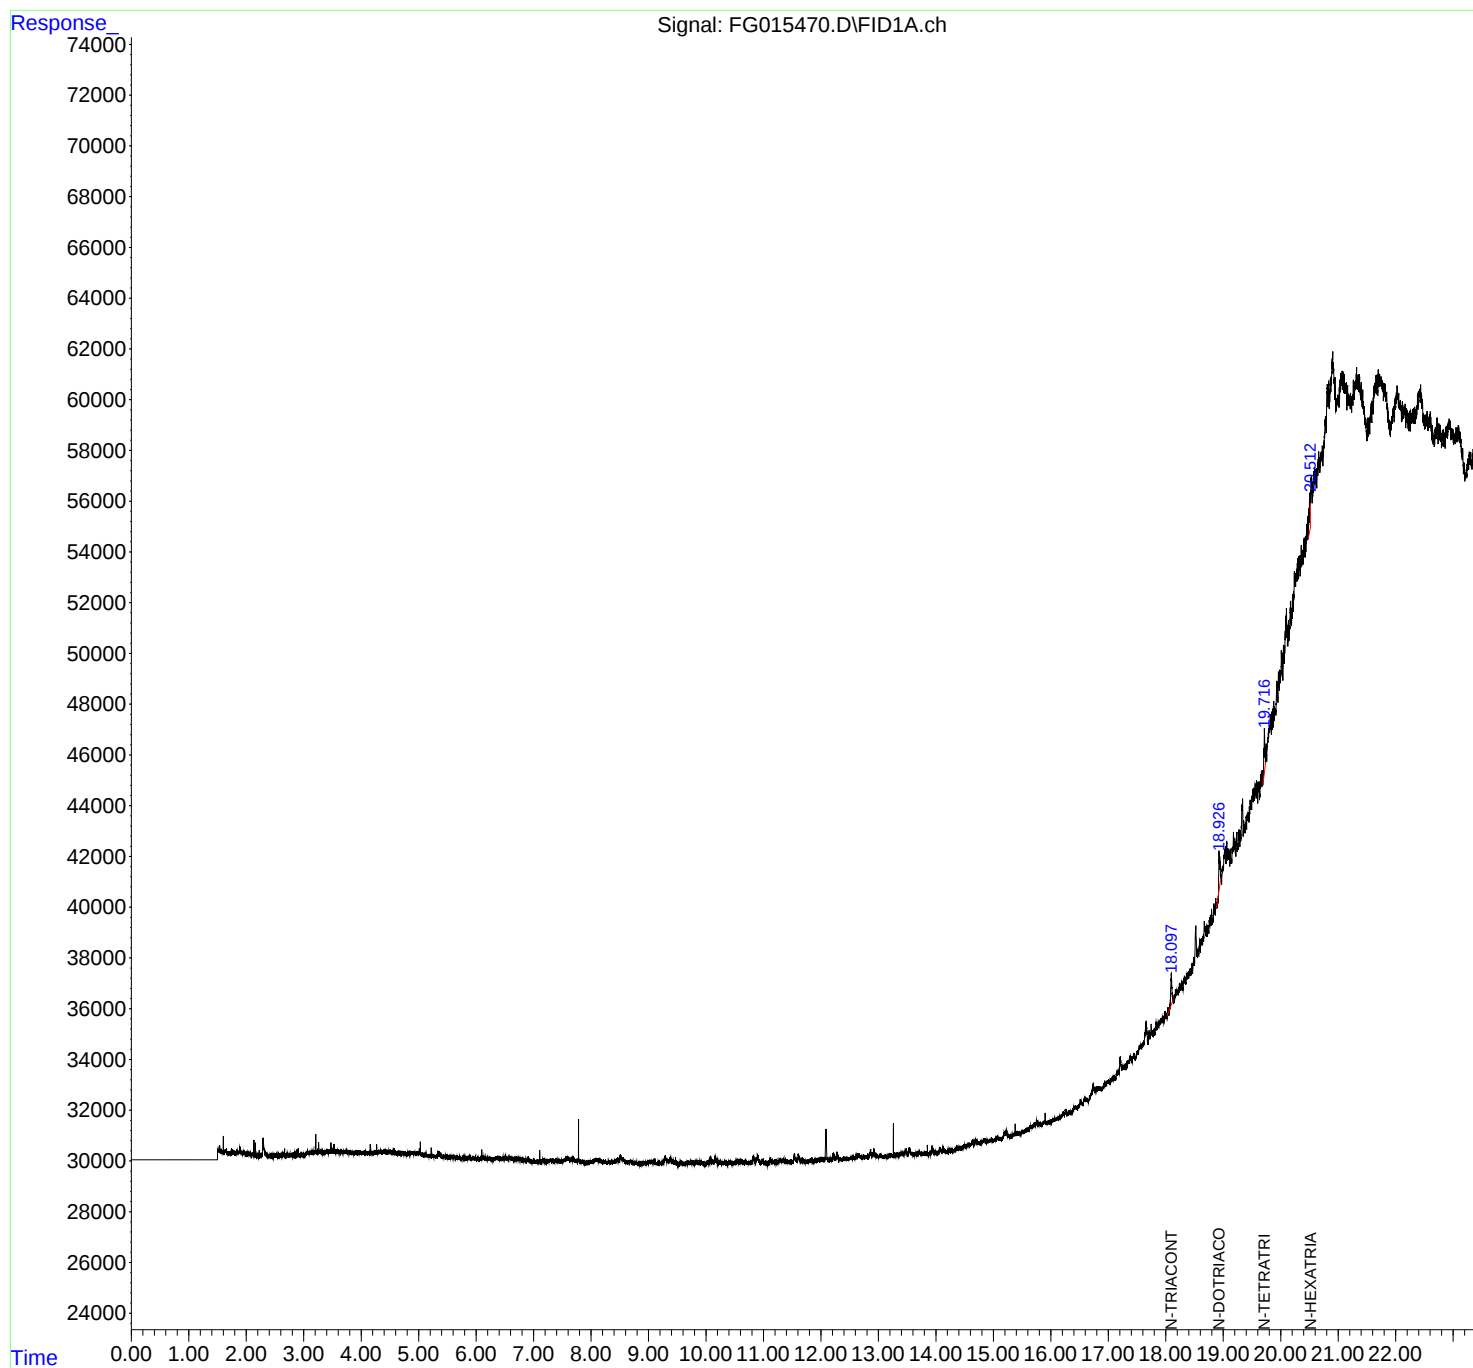


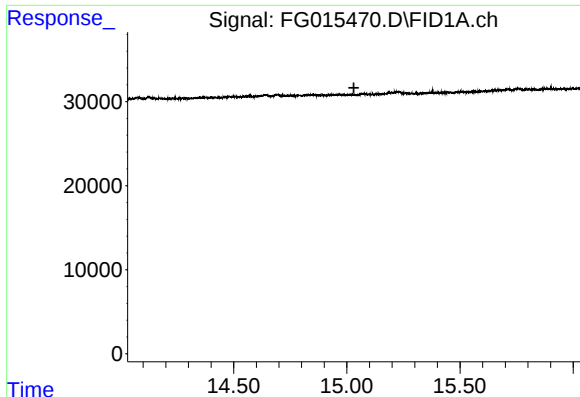

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 15.031 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

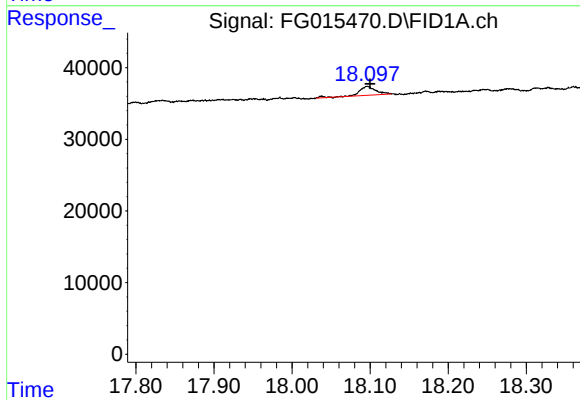


#13 N-TRIACONTANE

R.T.: 18.097 min
Delta R.T.: -0.003 min
Response: 18113
Conc: 0.16 ug/ml

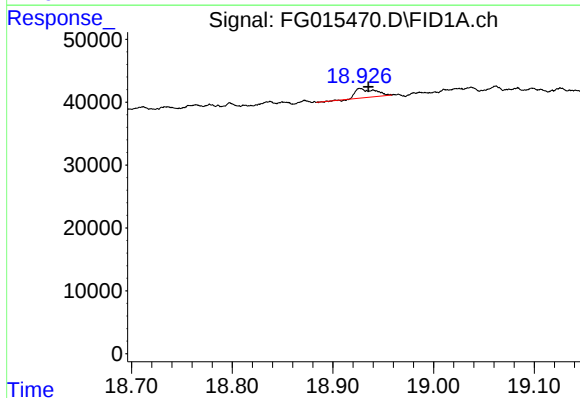


#14 N-DOTRIACONTANE

R.T.: 18.927 min
Delta R.T.: -0.008 min
Response: 18450
Conc: 0.16 ug/ml

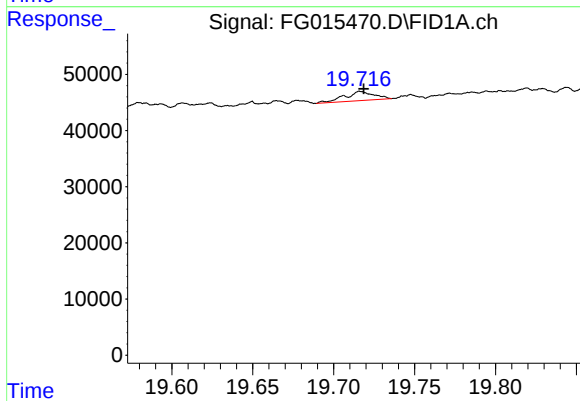

#15 N-TETRATRIACONTANE

R.T.: 19.717 min
Delta R.T.: -0.002 min
Response: 20433
Conc: 0.19 ug/ml

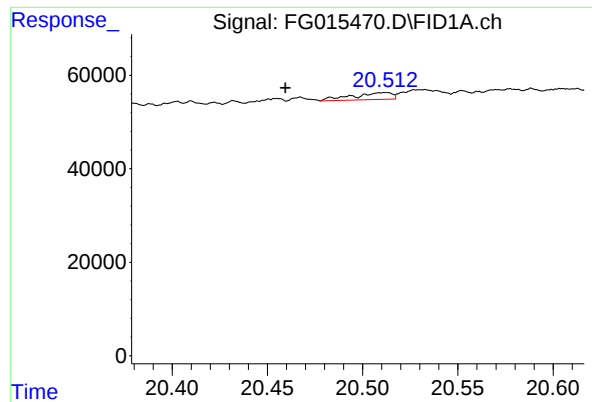

#16 N-HEXATRIACONTANE

R.T.: 20.512 min
Delta R.T.: 0.053 min
Response: 21234
Conc: 0.22 ug/ml

Instrument :

FID_G

ClientSampleId :