

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031225\
Data File : FG015477.D
Signal(s) : FID1A.ch
Acq On : 12 Mar 2025 15:25
Operator : YP\AJ
Sample : Q1502-19
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RR-DIES-WP

Integration File: autoint1.e
Quant Time: Mar 13 03:18:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030325.M
Quant Title :
QLast Update : Mon Mar 03 14:06:11 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.027	2328408	21.386 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031225\
Data File : FG015477.D
Signal(s) : FID1A.ch
Acq On : 12 Mar 2025 15:25
Operator : YP\AJ
Sample : Q1502-19
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RR-DIES-WP

Integration File: autoint1.e
Quant Time: Mar 13 03:18:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030325.M
Quant Title :
QLast Update : Mon Mar 03 14:06:11 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

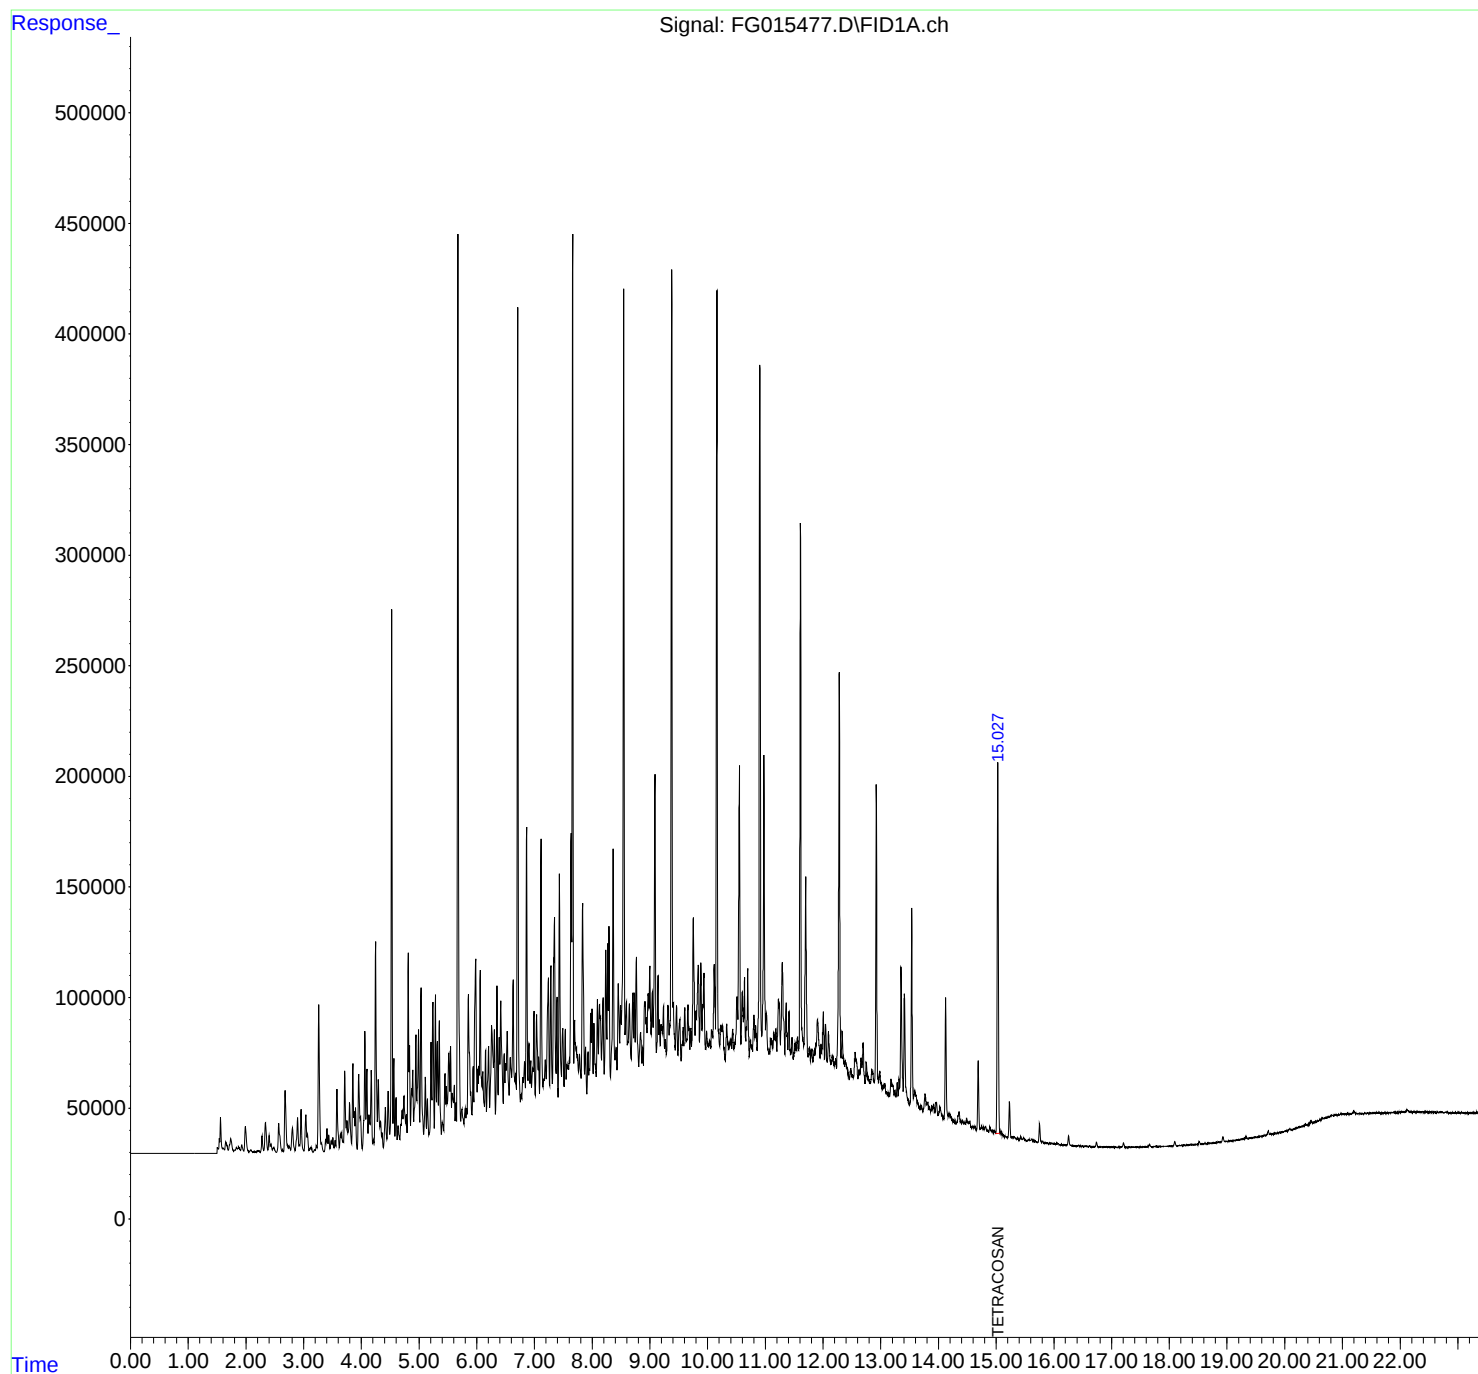

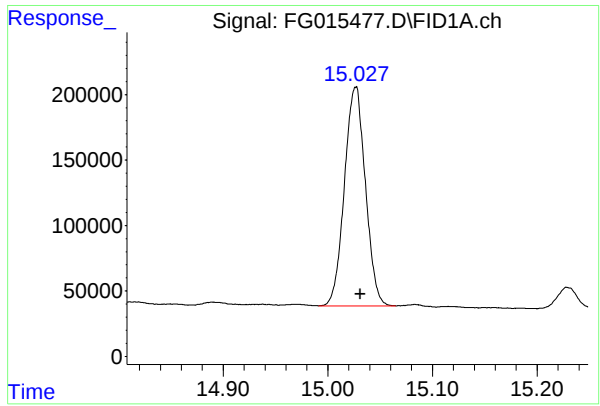

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.027 min
Delta R.T.: -0.004 min
Response: 2328408
Conc: 21.39 ug/ml

Instrument :
FID_G
ClientSampleId :
RR-DIES-WP