

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031319\
Data File : FG004157.D
Signal(s) : FID1A.ch
Acq On : 13 Mar 2019 10:52
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 13 13:35:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.188	3152739	23.256 ug/ml
12)	N-OCTACOSANE	16.611	2932849	21.422 ug/ml
13)	N-TRIACONTANE	17.498	297747	2.230 ug/ml
14)	N-DOTRIACONTANE	18.334	292985	2.316 ug/ml
15)	N-TETRATRIACONTANE	19.119	209508	1.768 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031319\
Data File : FG004157.D
Signal(s) : FID1A.ch
Acq On : 13 Mar 2019 10:52
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 13 13:35:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

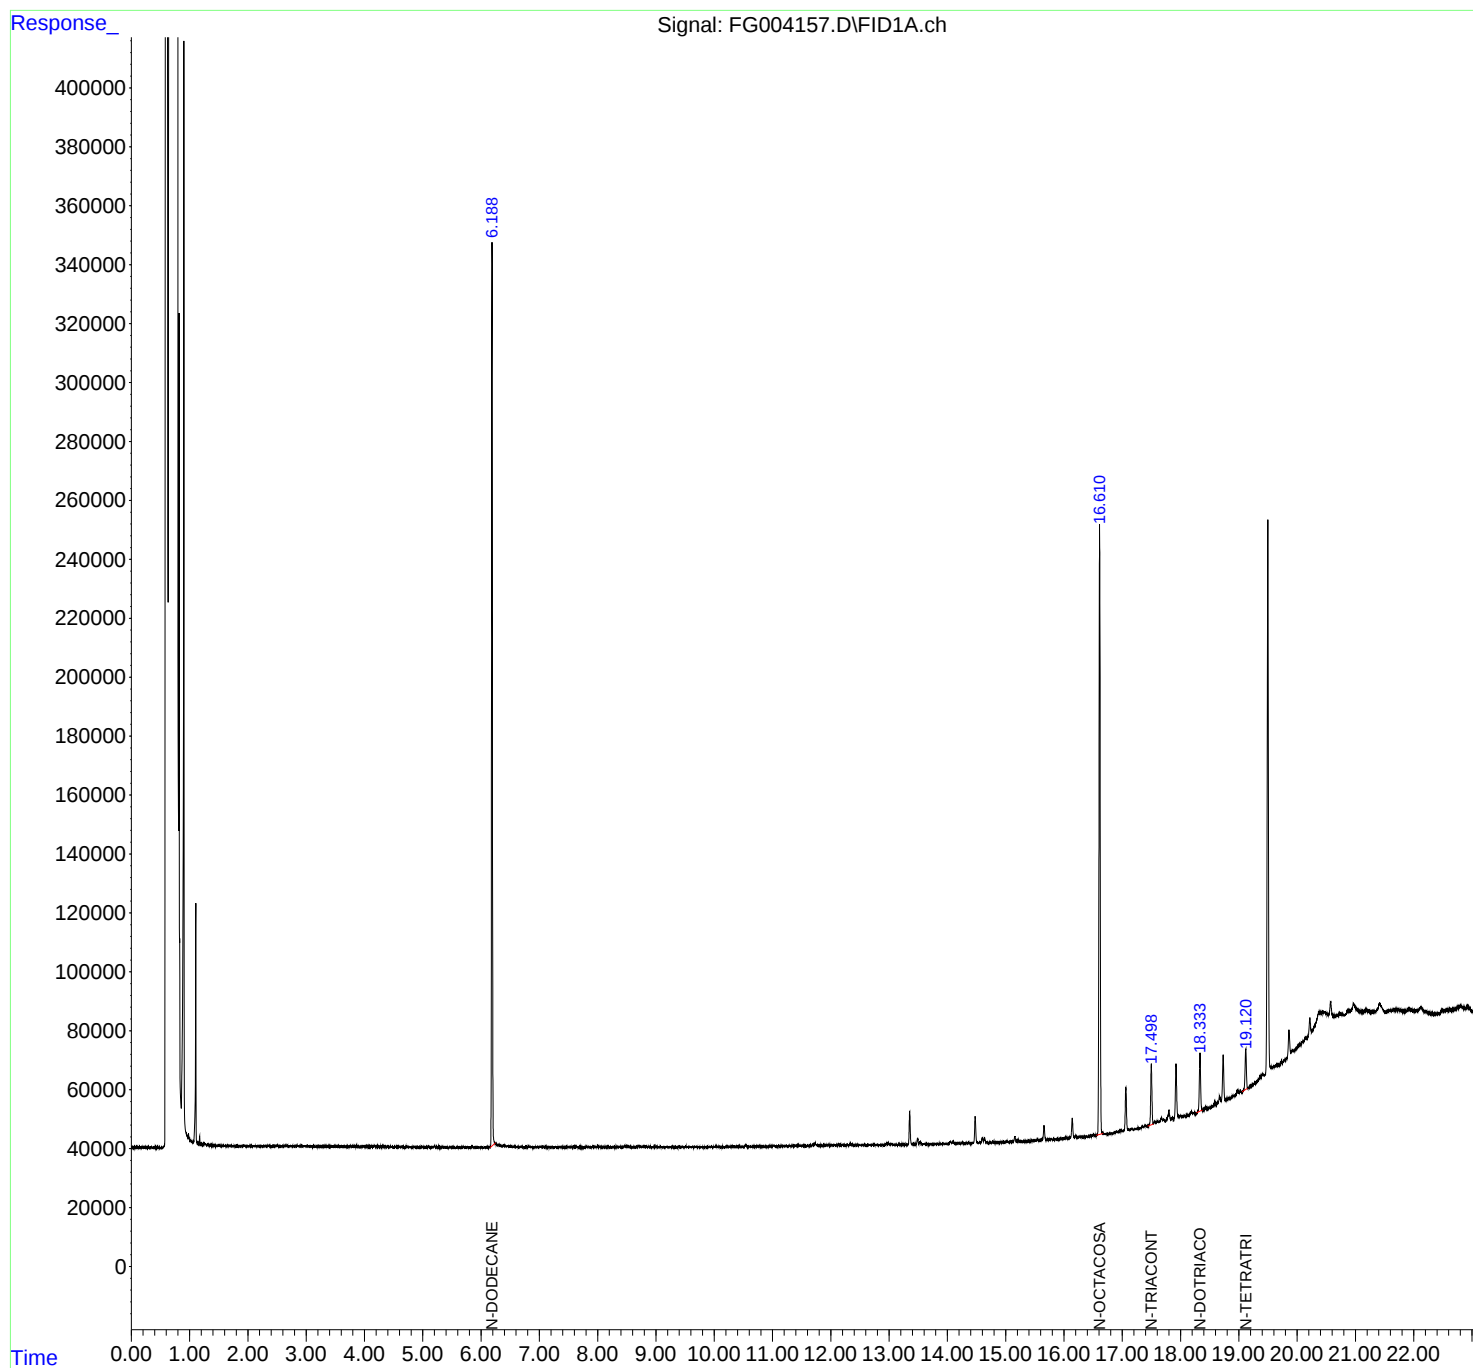


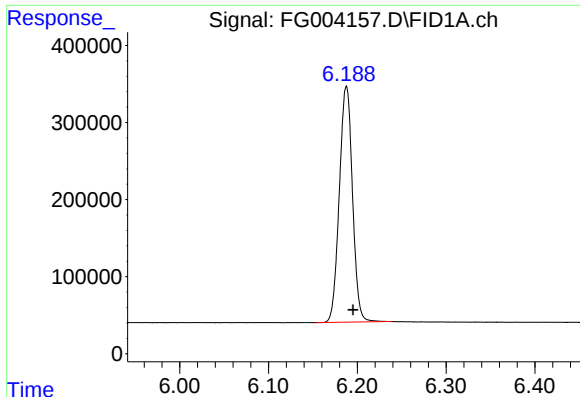

#3 N-DODECANE


R.T.: 6.188 min
Delta R.T.: -0.007 min
Response: 3152739
Conc: 23.26 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

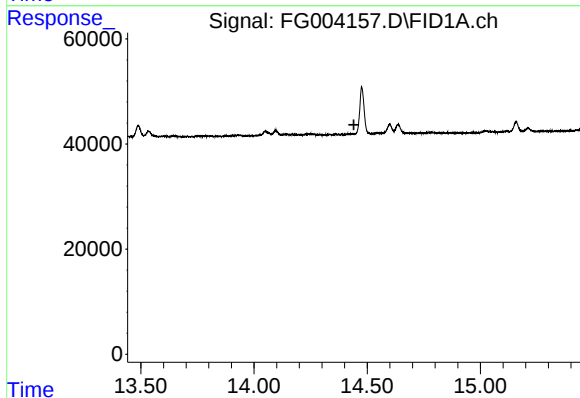


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.441 min
Response: 0
Conc: N.D.

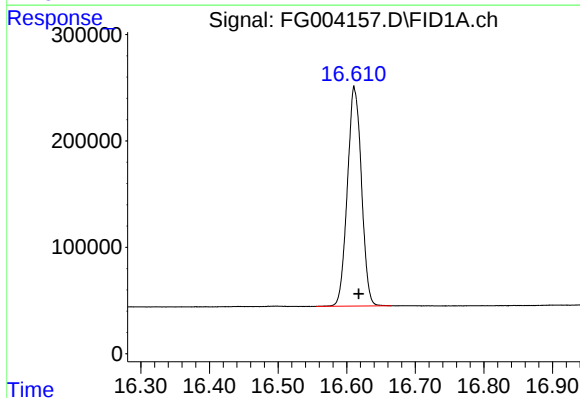


#12 N-OCTACOSANE

R.T.: 16.611 min
Delta R.T.: -0.006 min
Response: 2932849
Conc: 21.42 ug/ml

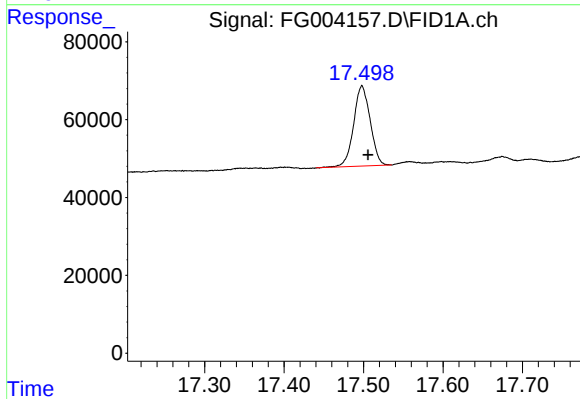

#13 N-TRIACONTANE


R.T.: 17.498 min
Delta R.T.: -0.008 min
Response: 297747
Conc: 2.23 ug/ml

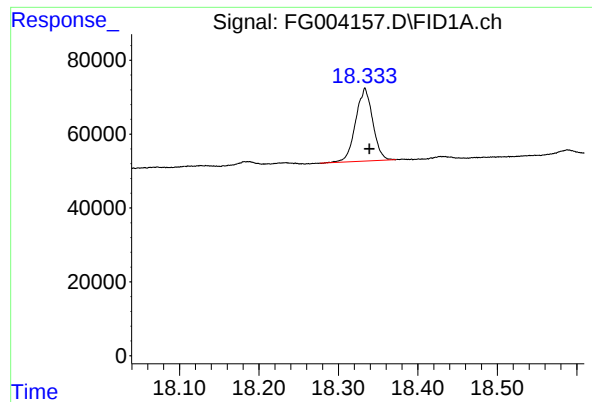

#14 N-DOTRIACONTANE

R.T.: 18.334 min
Delta R.T.: -0.006 min
Response: 292985
Conc: 2.32 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

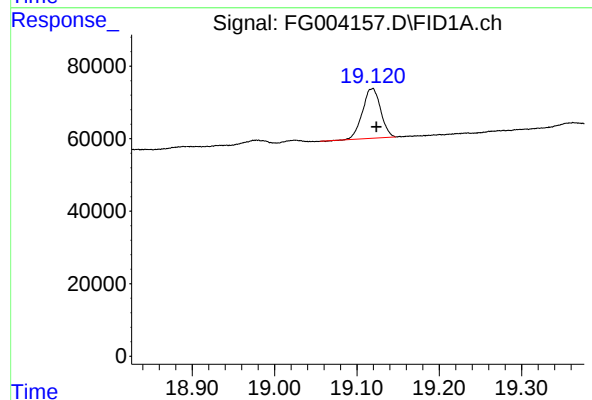

#15 N-TETRATRIACONTANE

R.T.: 19.119 min
Delta R.T.: -0.005 min
Response: 209508
Conc: 1.77 ug/ml