

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031319\
Data File : FG004165.D
Signal(s) : FID1A.ch
Acq On : 13 Mar 2019 16:13
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 14 01:27:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.188	3128859	23.080 ug/ml
12)	N-OCTACOSANE	16.609	3029052	22.124 ug/ml
13)	N-TRIACONTANE	17.496	324891	2.433 ug/ml
14)	N-DOTRIACONTANE	18.329	346253	2.737 ug/ml
15)	N-TETRATRIACONTANE	19.115	253093	2.136 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031319\
Data File : FG004165.D
Signal(s) : FID1A.ch
Acq On : 13 Mar 2019 16:13
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 14 01:27:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

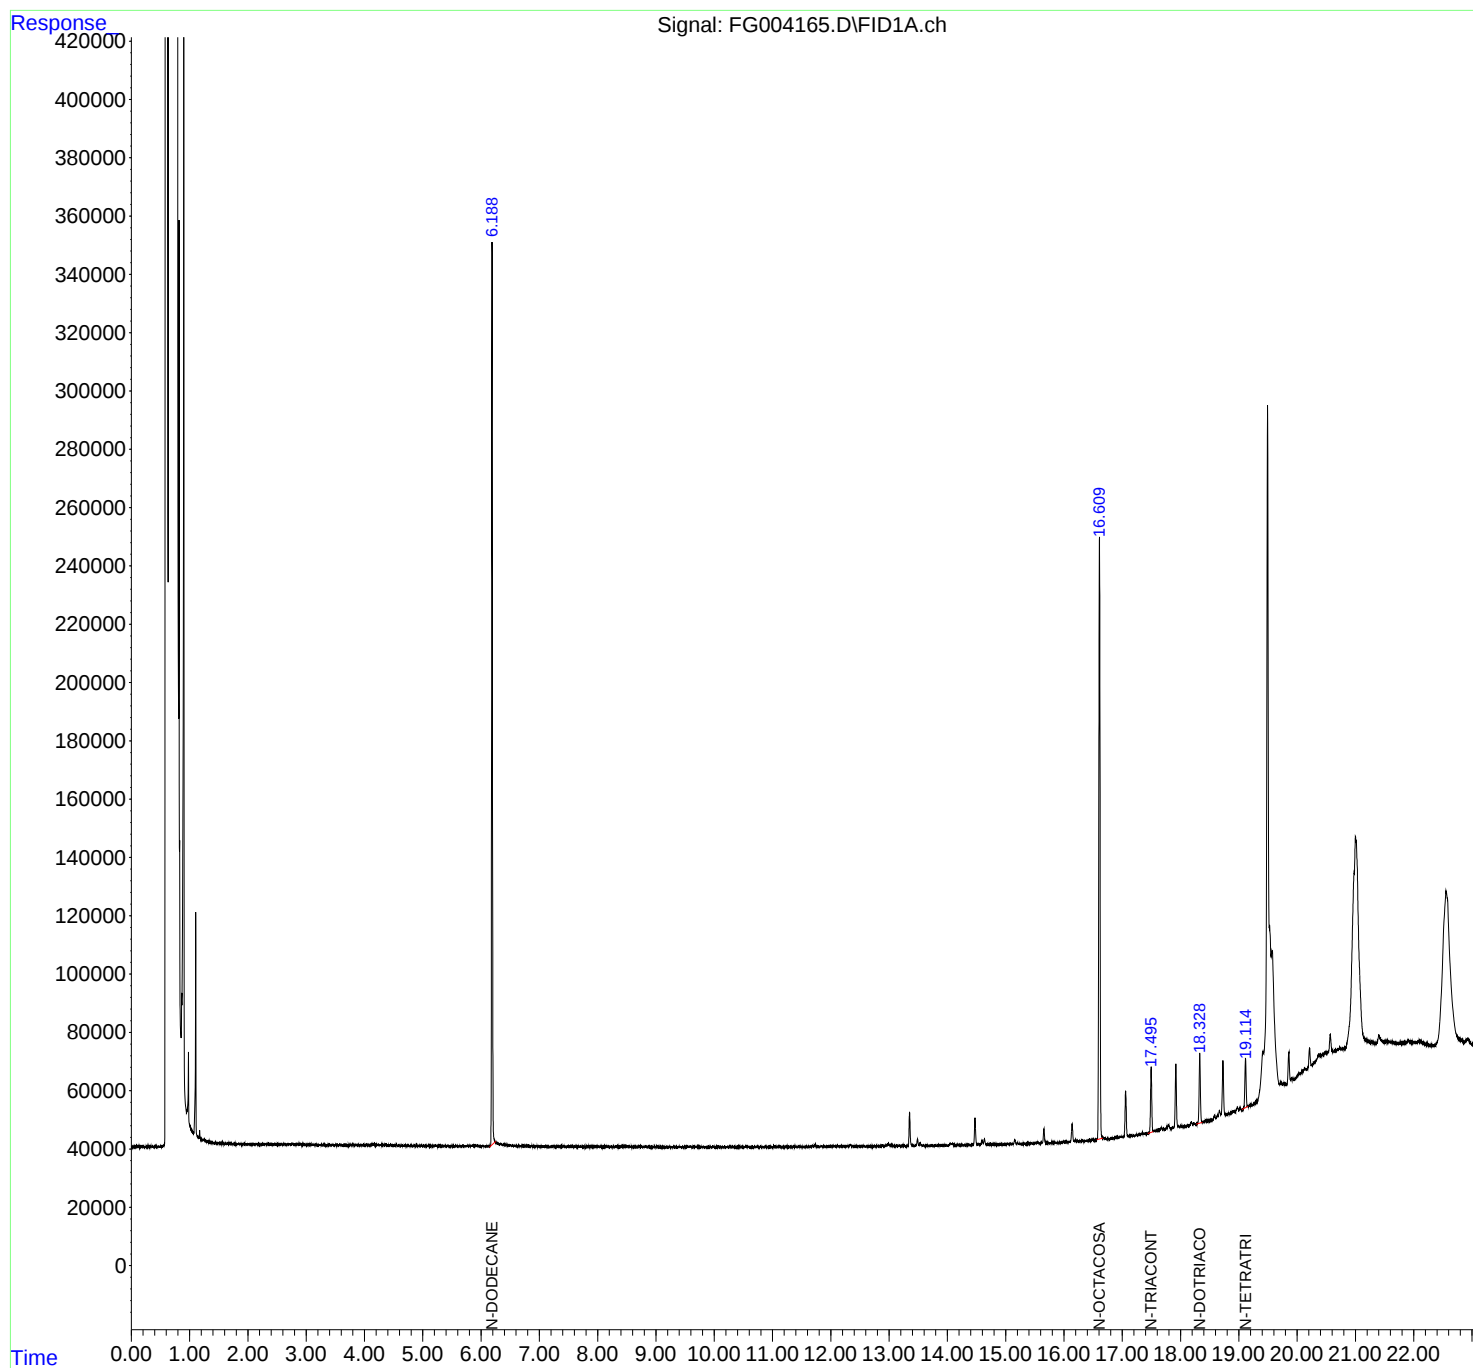


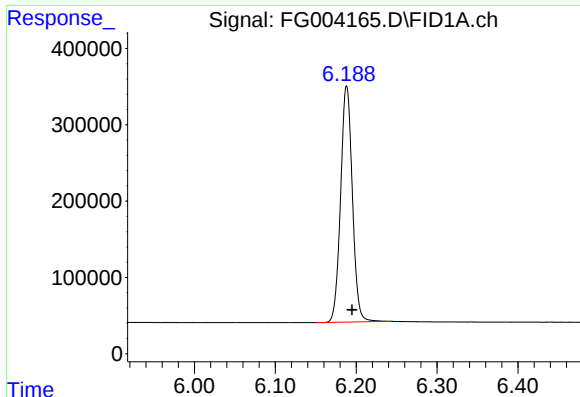

#3 N-DODECANE


R.T.: 6.188 min
Delta R.T.: -0.007 min
Response: 3128859
Conc: 23.08 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

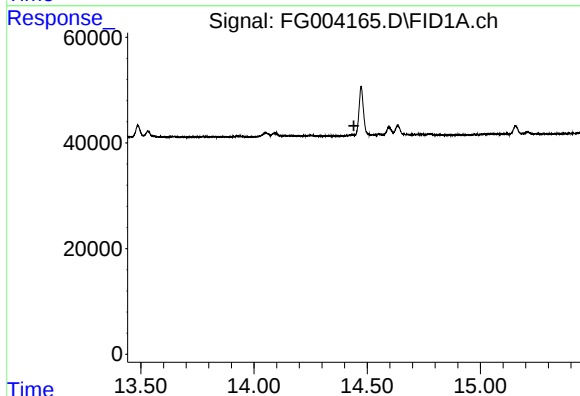


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.441 min
Response: 0
Conc: N.D.

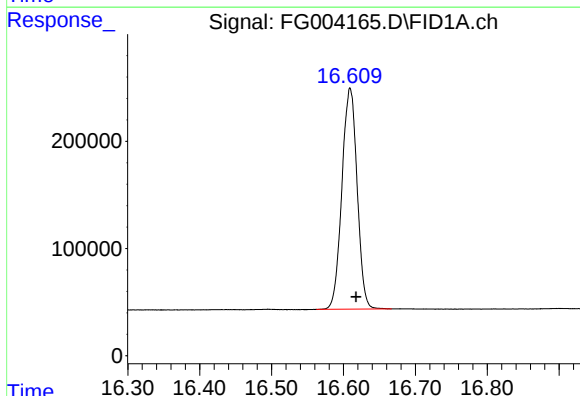


#12 N-OCTACOSANE

R.T.: 16.609 min
Delta R.T.: -0.008 min
Response: 3029052
Conc: 22.12 ug/ml

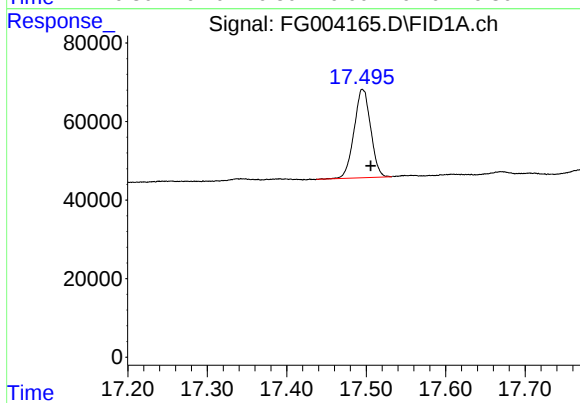

#13 N-TRIACONTANE


R.T.: 17.496 min
Delta R.T.: -0.010 min
Response: 324891
Conc: 2.43 ug/ml

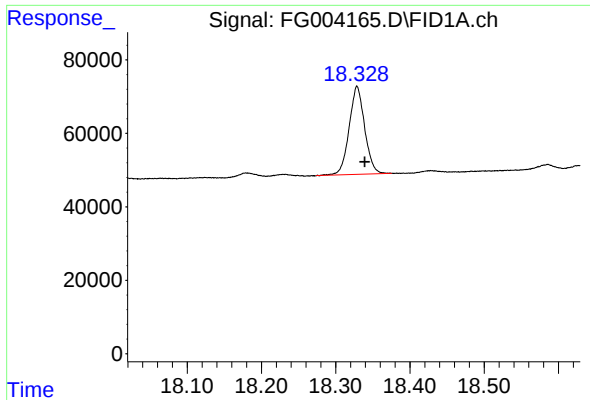

#14 N-DOTRIACONTANE

R.T.: 18.329 min
Delta R.T.: -0.010 min
Response: 346253
Conc: 2.74 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

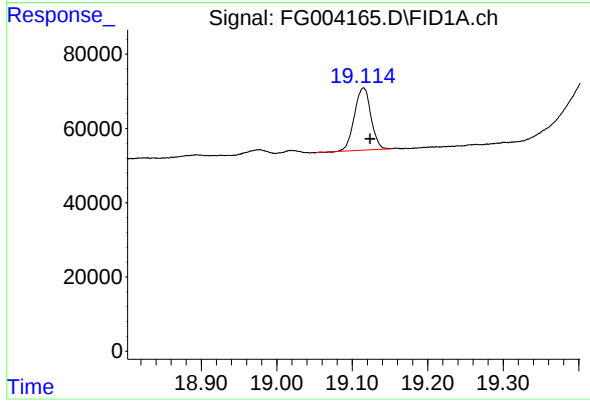

#15 N-TETRATRIACONTANE

R.T.: 19.115 min
Delta R.T.: -0.009 min
Response: 253093
Conc: 2.14 ug/ml