

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031319\
Data File : FG004166.D
Signal(s) : FID1A.ch
Acq On : 13 Mar 2019 16:48
Operator : AJ\SJ
Sample : K1687-01 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
HR-06-031119-A

Integration File: autoint1.e
Quant Time: Mar 14 01:27:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.432	310529	2.470 ug/ml
Target Compounds			
2) N-DECANE	4.164	628839	4.703 ug/ml
3) N-DODECANE	6.187	2054114	15.152 ug/ml
4) N-TETRADECANE	7.981	1250374	8.967 ug/ml
5) N-HEXADECANE	9.581	467791	3.287 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031319\
Data File : FG004166.D
Signal(s) : FID1A.ch
Acq On : 13 Mar 2019 16:48
Operator : AJ\SJ
Sample : K1687-01 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
HR-06-031119-A

Integration File: autoint1.e
Quant Time: Mar 14 01:27:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

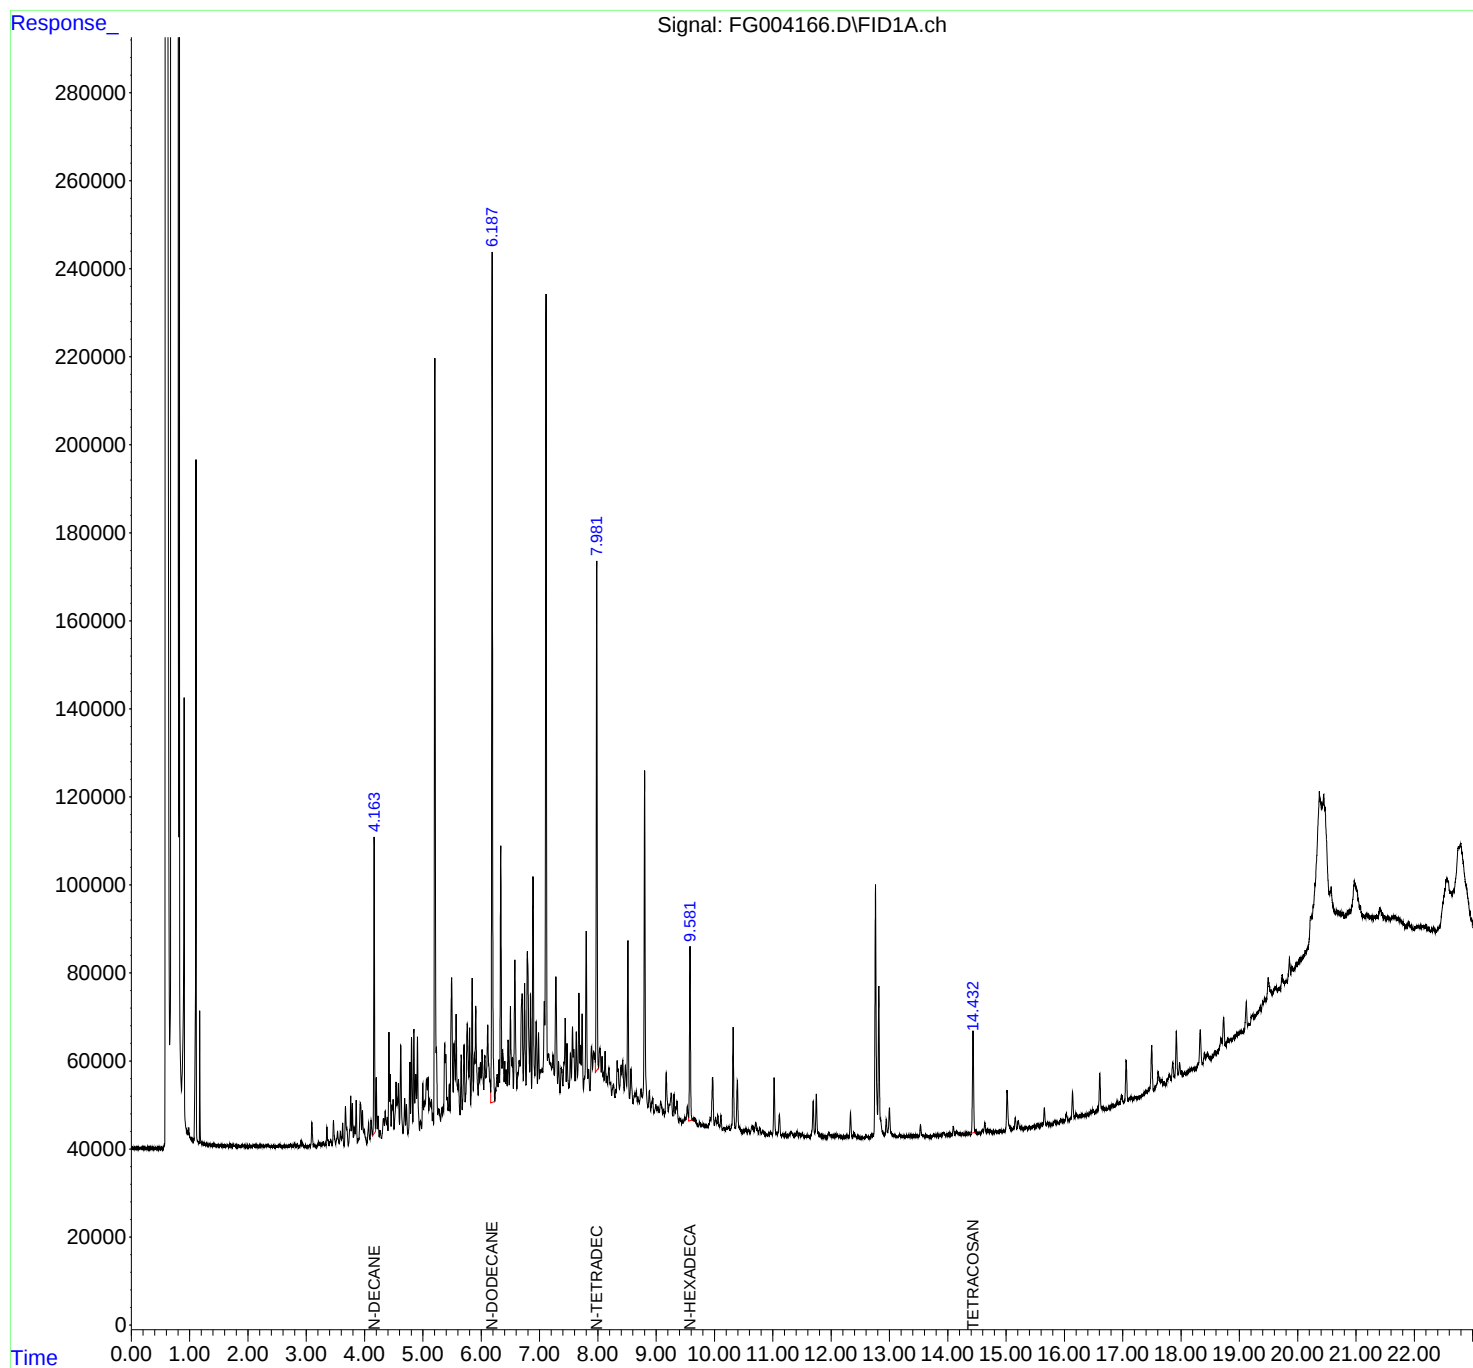


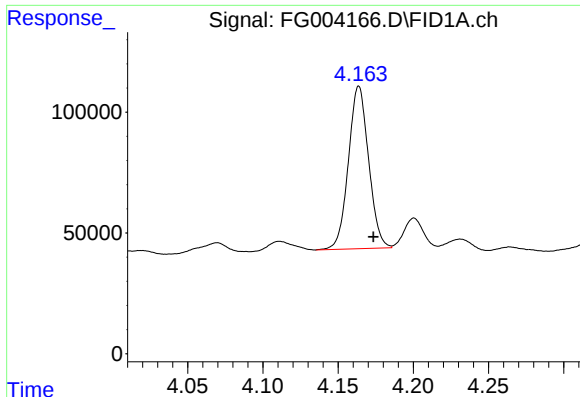

#2 N-DECANE


R.T.: 4.164 min
Delta R.T.: -0.010 min
Response: 628839
Conc: 4.70 ug/ml

Instrument :
FID_G
ClientSampleId :
HR-06-031119-A

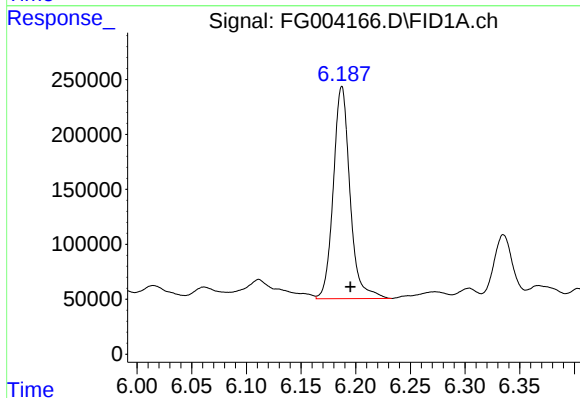


#3 N-DODECANE

R.T.: 6.187 min
Delta R.T.: -0.008 min
Response: 2054114
Conc: 15.15 ug/ml

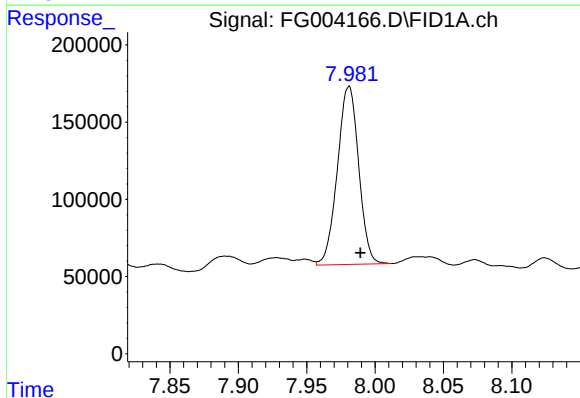


#4 N-TETRADECANE

R.T.: 7.981 min
Delta R.T.: -0.008 min
Response: 1250374
Conc: 8.97 ug/ml

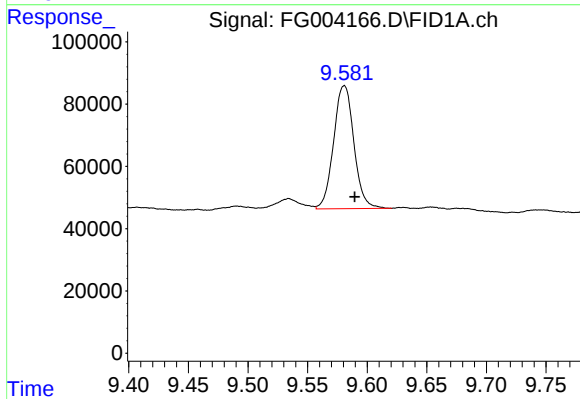

#5 N-HEXADECANE

R.T.: 9.581 min
Delta R.T.: -0.009 min
Response: 467791
Conc: 3.29 ug/ml

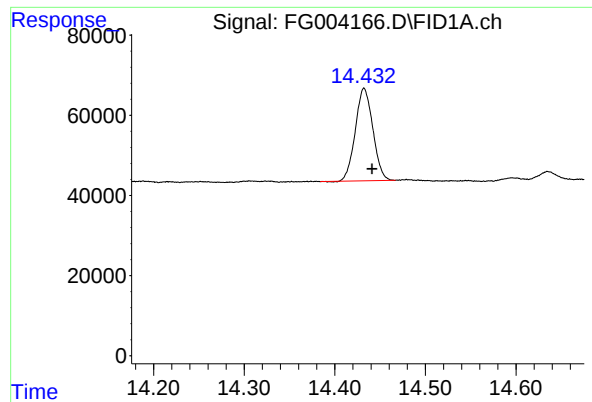

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.432 min
Delta R.T.: -0.009 min
Response: 310529
Conc: 2.47 ug/ml

Instrument :
FID_G
ClientSampleId :
HR-06-031119-A