

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031319\
 Data File : FG004170.D
 Signal(s) : FID1A.ch
 Acq On : 13 Mar 2019 18:50
 Operator : AJ\SJ
 Sample : K1693-05 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 OR-02-031219-A

Integration File: autoint1.e
 Quant Time: Mar 14 01:28:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
 Quant Title :
 QLast Update : Tue Mar 05 03:05:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.435	397881	3.165 ug/ml
Target Compounds			
7) N-EICOSANE	12.378	3871743	27.102 ug/ml
8) N-DOCOSANE	13.542	378638	2.668 ug/ml
10) N-TETRACOSANE	14.601	2244870	15.918 ug/ml
11) N-HEXACOSANE	15.659	228166	1.638 ug/ml
12) N-OCTACOSANE	16.610	542345	3.961 ug/ml
14) N-DOTRIACONTANE	18.282f	853446	6.745 ug/ml
15) N-TETRATRIACONTANE	19.119	371388	3.134 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031319\
Data File : FG004170.D
Signal(s) : FID1A.ch
Acq On : 13 Mar 2019 18:50
Operator : AJ\SJ
Sample : K1693-05 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
OR-02-031219-A

Integration File: autoint1.e
Quant Time: Mar 14 01:28:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

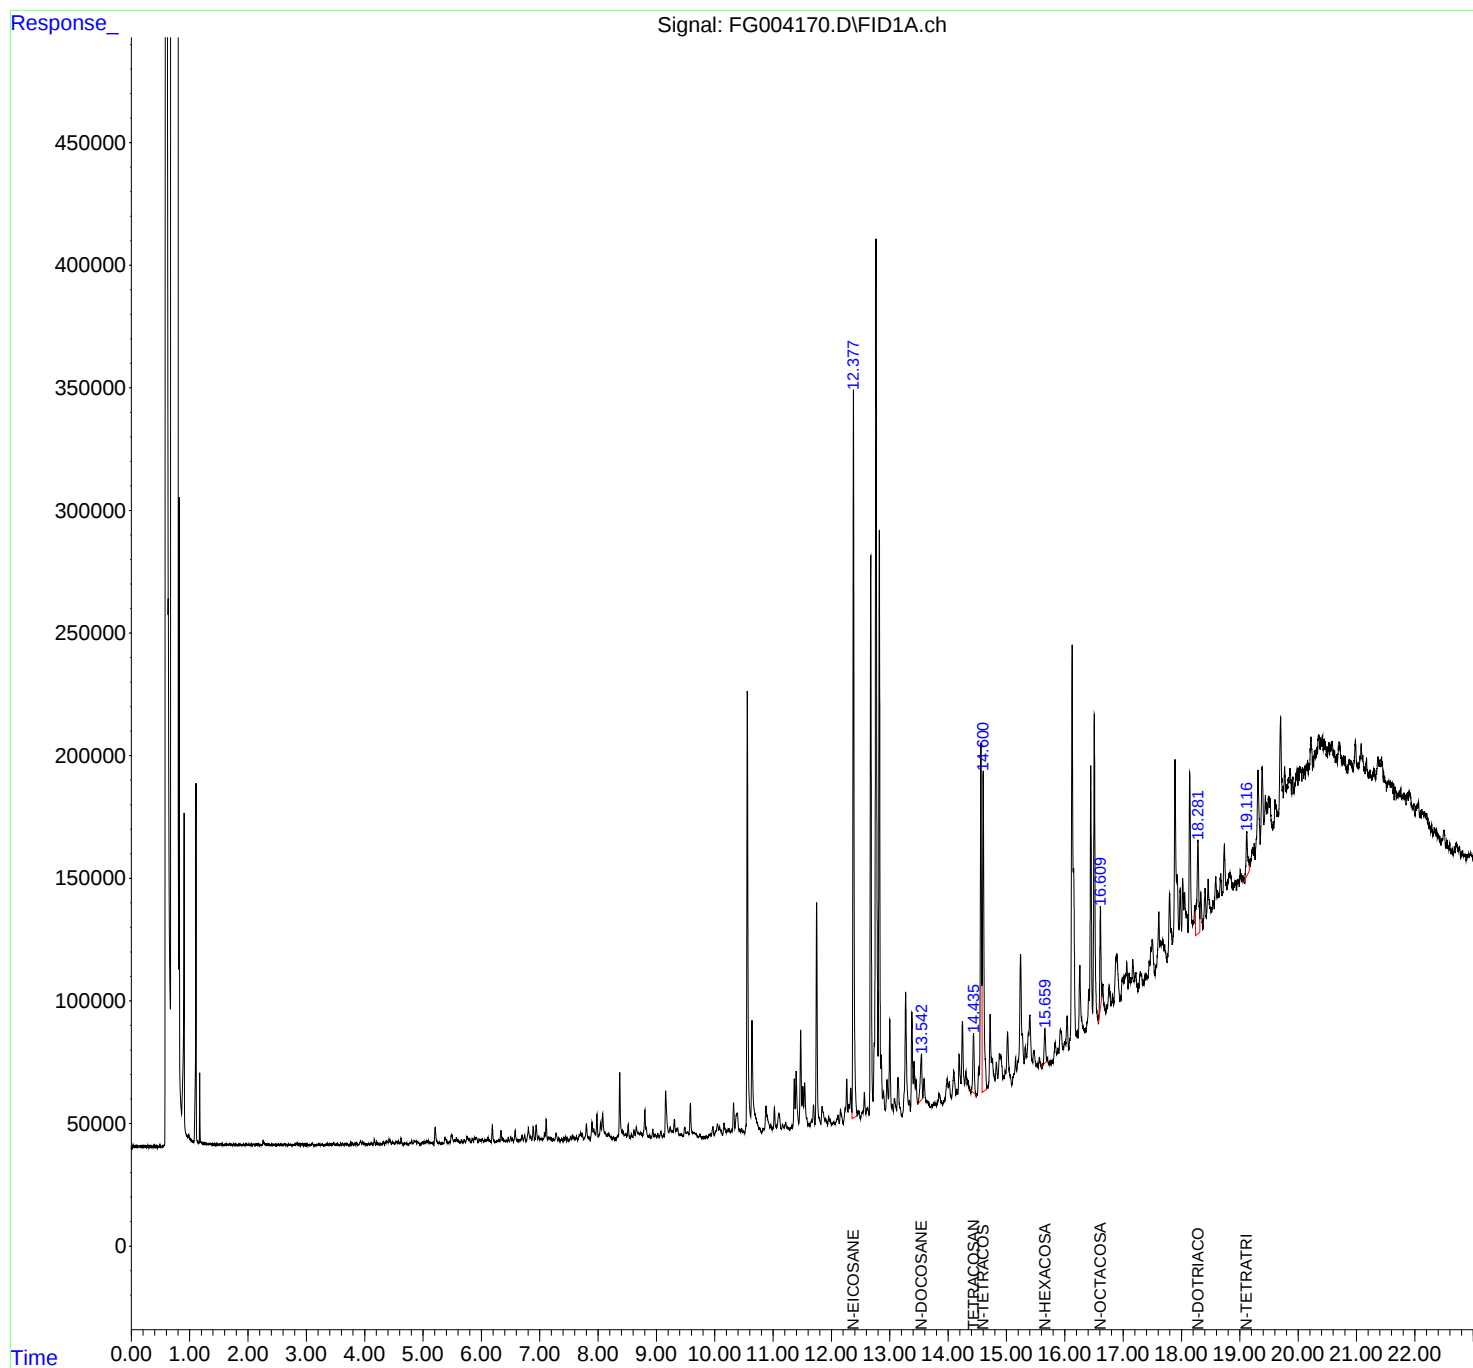


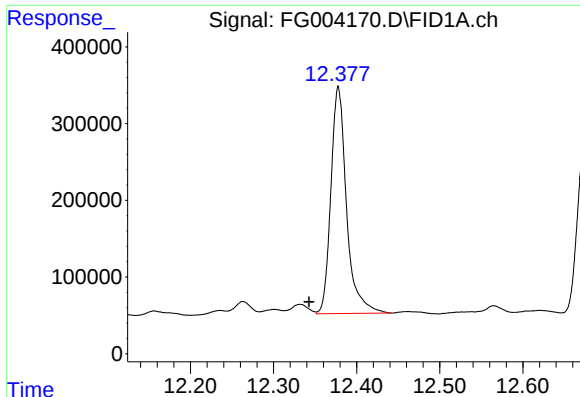

#7 N-EICOSANE


R.T.: 12.378 min
Delta R.T.: 0.035 min
Response: 3871743
Conc: 27.10 ug/ml

Instrument :
FID_G
ClientSampleId :
OR-02-031219-A

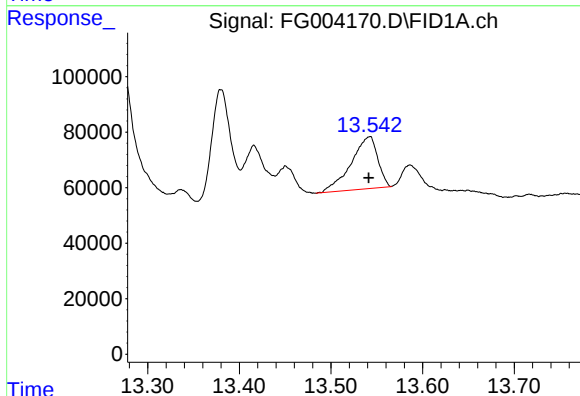


#8 N-DOCOSANE

R.T.: 13.542 min
Delta R.T.: 0.001 min
Response: 378638
Conc: 2.67 ug/ml

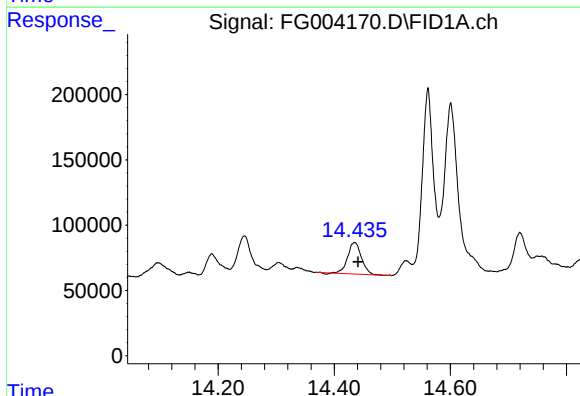


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.435 min
Delta R.T.: -0.006 min
Response: 397881
Conc: 3.16 ug/ml

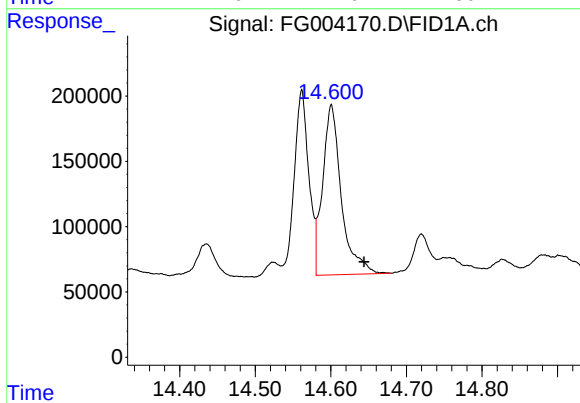

#10 N-TETRACOSANE


R.T.: 14.601 min
Delta R.T.: -0.043 min
Response: 2244870
Conc: 15.92 ug/ml

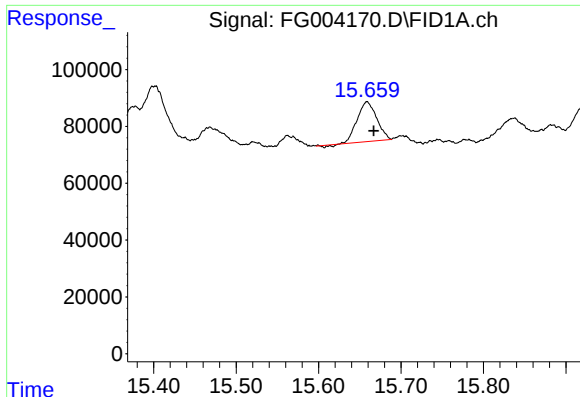

#11 N-HEXACOSANE


R.T.: 15.659 min
Delta R.T.: -0.008 min
Response: 228166
Conc: 1.64 ug/ml

Instrument :
FID_G
ClientSampleId :
OR-02-031219-A

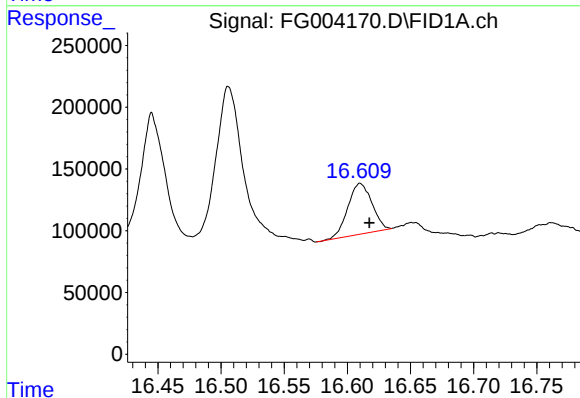


#12 N-OCTACOSANE

R.T.: 16.610 min
Delta R.T.: -0.007 min
Response: 542345
Conc: 3.96 ug/ml

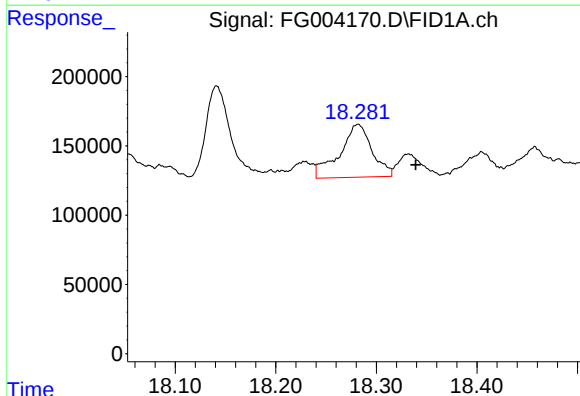

#14 N-DOTRIACONTANE

R.T.: 18.282 min
Delta R.T.: -0.057 min
Response: 853446
Conc: 6.74 ug/ml

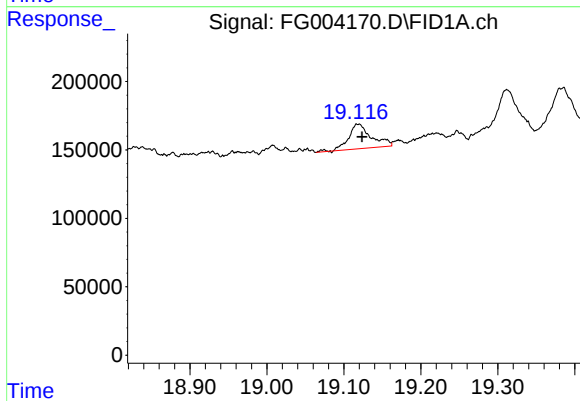

#15 N-TETRATRIACONTANE

R.T.: 19.119 min
Delta R.T.: -0.005 min
Response: 371388
Conc: 3.13 ug/ml