

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031323\
Data File : FG011573.D
Signal(s) : FID1A.ch
Acq On : 13 Mar 2023 17:20
Operator : YP\AJ
Sample : 01870-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RAW-WATER

Integration File: autoint1.e
Quant Time: Mar 14 02:31:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG022123.M
Quant Title :
QLast Update : Tue Feb 21 16:44:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.057	1714361	16.299 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031323\
Data File : FG011573.D
Signal(s) : FID1A.ch
Acq On : 13 Mar 2023 17:20
Operator : YP\AJ
Sample : 01870-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RAW-WATER

Integration File: autoint1.e
Quant Time: Mar 14 02:31:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG022123.M
Quant Title :
QLast Update : Tue Feb 21 16:44:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

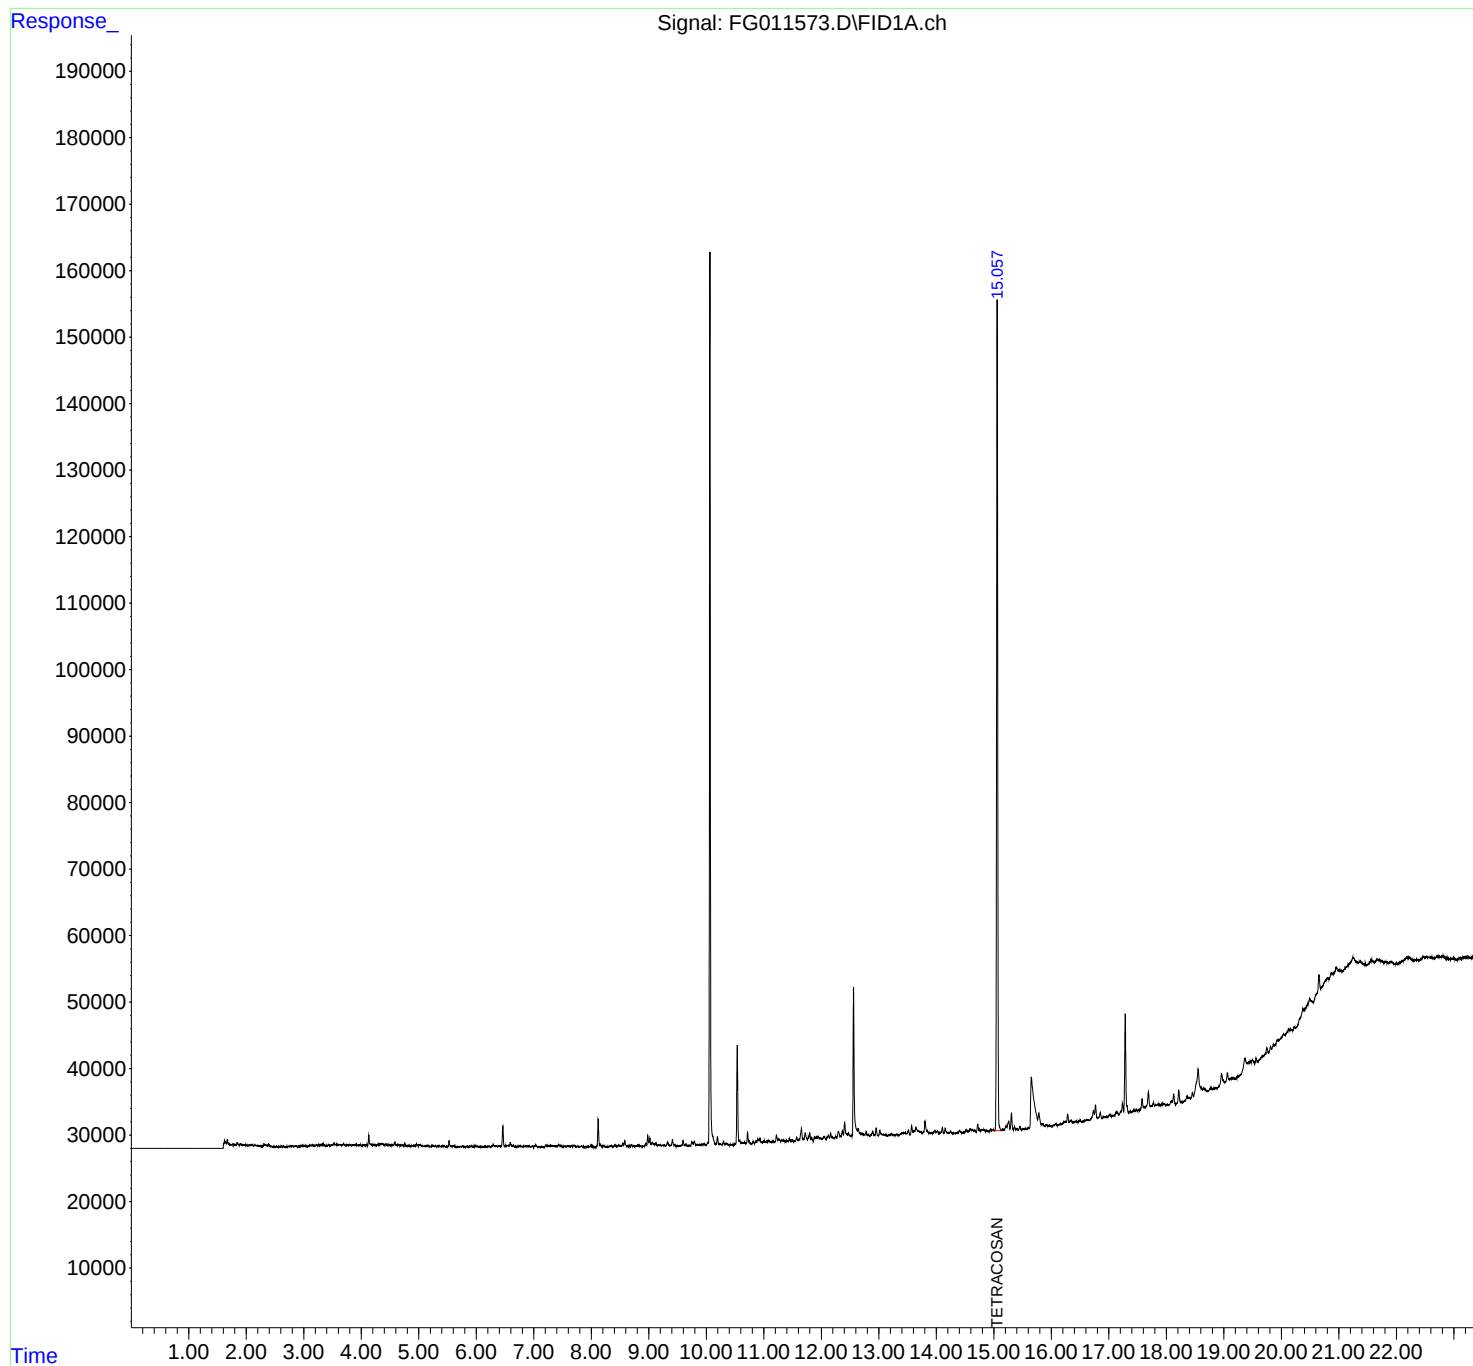

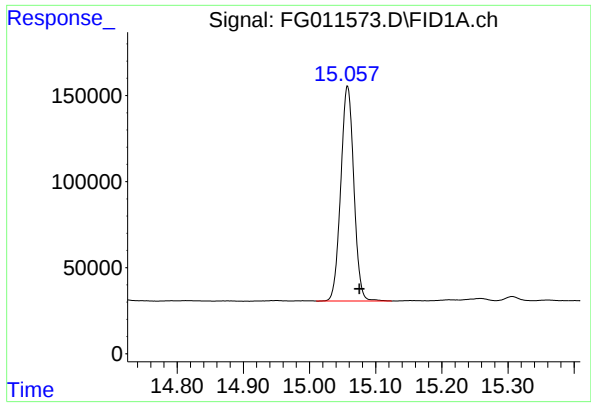

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.057 min
Delta R.T.: -0.018 min
Response: 1714361
Conc: 16.30 ug/ml

Instrument :
FID_G
ClientSampleId :
RAW-WATER