

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031419\
 Data File : FG004184.D
 Signal(s) : FID1A.ch
 Acq On : 14 Mar 2019 11:29
 Operator : AJ\SJ
 Sample : K1870-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 14 14:15:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
 Quant Title :
 QLast Update : Tue Mar 05 03:05:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.434	1236284	9.834 ug/ml
Target Compounds			
4) N-TETRADECANE	8.042f	148890	1.068 ug/ml
7) N-EICOSANE	12.379	629971	4.410 ug/ml
10) N-TETRACOSANE	14.602	577152	4.092 ug/ml
12) N-OCTACOSANE	16.612	313324	2.289 ug/ml
13) N-TRIACONTANE	17.502	663528	4.969 ug/ml
14) N-DOTRIACONTANE	18.334	397764	3.144 ug/ml
15) N-TETRATRIACONTANE	19.124	598144	5.048 ug/ml
16) N-HEXATRIACONTANE	19.875	532209	4.807 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031419\
Data File : FG004184.D
Signal(s) : FID1A.ch
Acq On : 14 Mar 2019 11:29
Operator : AJ\SJ
Sample : K1870-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 14 14:15:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

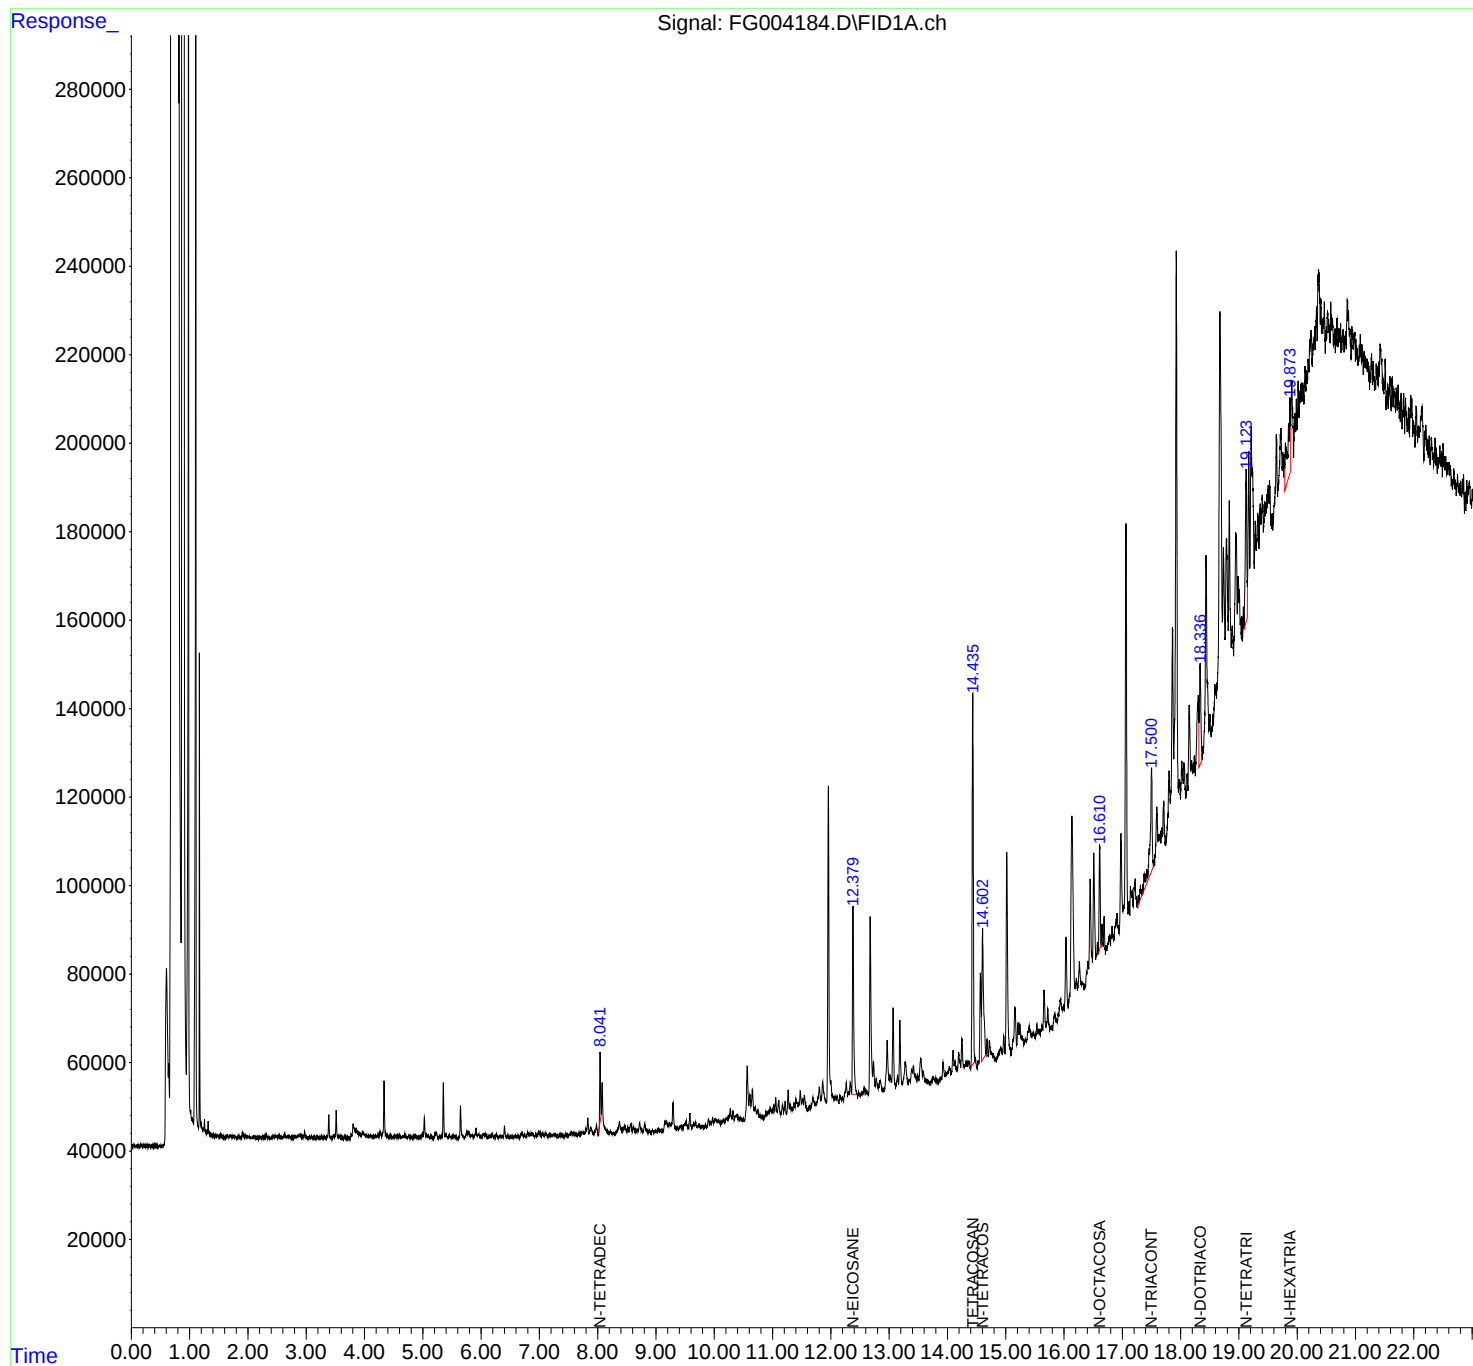


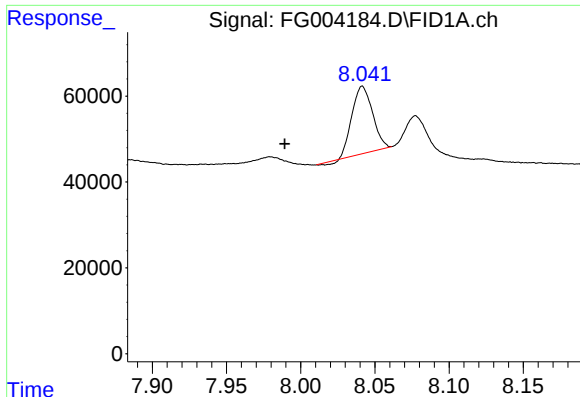

#4 N-TETRADECANE


R.T.: 8.042 min
Delta R.T.: 0.052 min
Response: 148890
Conc: 1.07 ug/ml

Instrument :
FID_G
ClientSampleId :

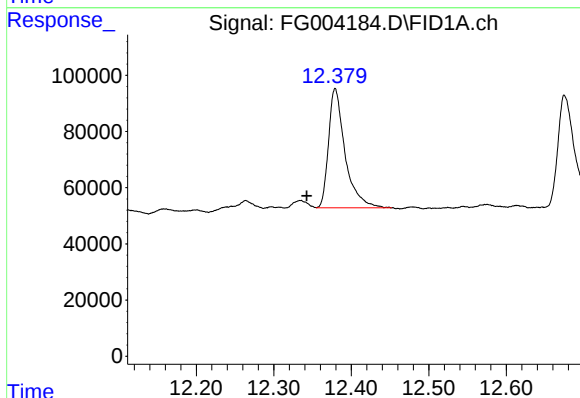


#7 N-EICOSANE

R.T.: 12.379 min
Delta R.T.: 0.037 min
Response: 629971
Conc: 4.41 ug/ml

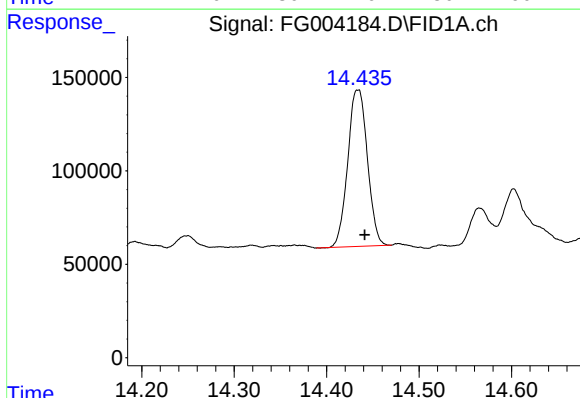


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.434 min
Delta R.T.: -0.007 min
Response: 1236284
Conc: 9.83 ug/ml

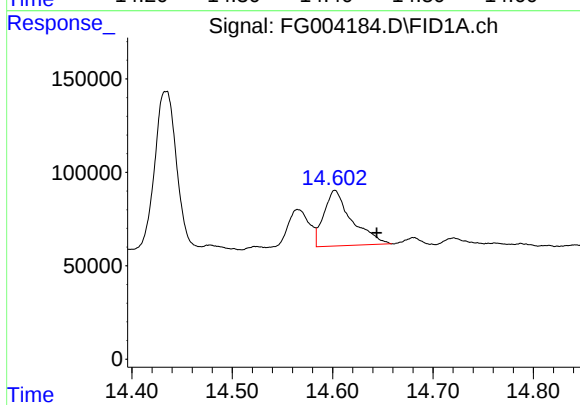

#10 N-TETRACOSANE


R.T.: 14.602 min
Delta R.T.: -0.041 min
Response: 577152
Conc: 4.09 ug/ml

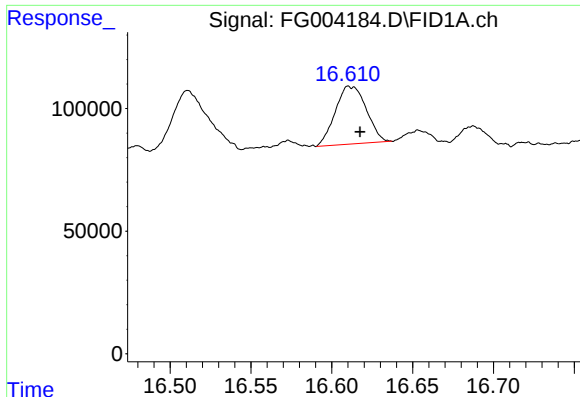

#12 N-OCTACOSANE


R.T.: 16.612 min
Delta R.T.: -0.006 min
Response: 313324
Conc: 2.29 ug/ml

Instrument :
FID_G
ClientSampleId :

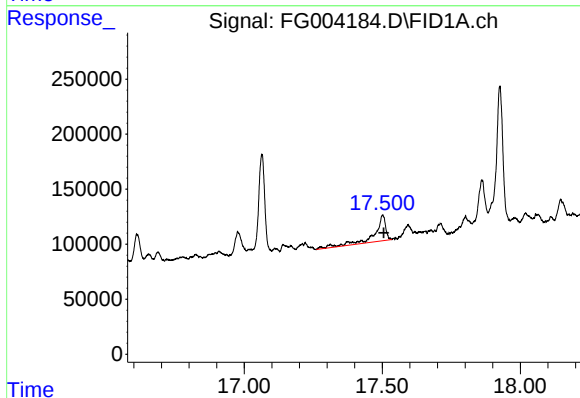


#13 N-TRIACONTANE

R.T.: 17.502 min
Delta R.T.: -0.004 min
Response: 663528
Conc: 4.97 ug/ml

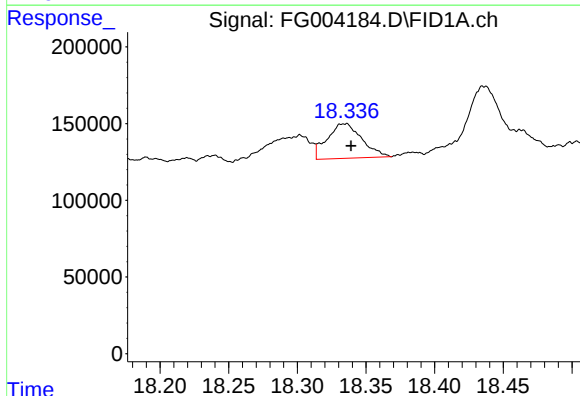


#14 N-DOTRIACONTANE

R.T.: 18.334 min
Delta R.T.: -0.005 min
Response: 397764
Conc: 3.14 ug/ml

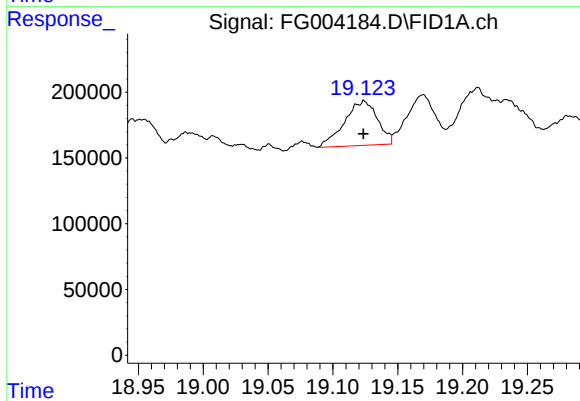

#15 N-TETRATRIACONTANE

R.T.: 19.124 min
Delta R.T.: 0.000 min
Response: 598144
Conc: 5.05 ug/ml

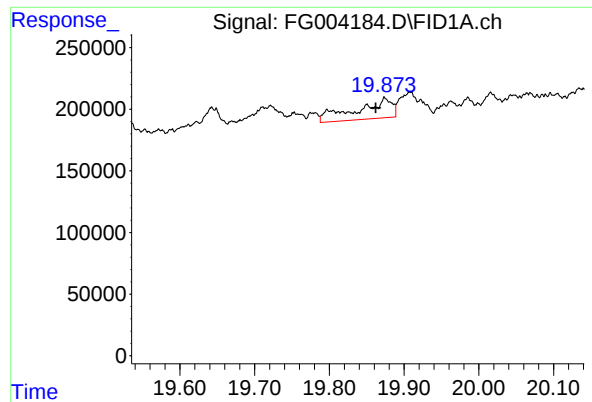

#16 N-HEXATRIACONTANE

R.T.: 19.875 min
Delta R.T.: 0.013 min
Response: 532209
Conc: 4.81 ug/ml

Instrument :
FID_G
ClientSampleId :