

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031419\
 Data File : FG004185.D
 Signal(s) : FID1A.ch
 Acq On : 14 Mar 2019 12:00
 Operator : AJ\SJ
 Sample : K1870-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 14 14:15:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
 Quant Title :
 QLast Update : Tue Mar 05 03:05:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.437	1556343	12.379 ug/ml
Target Compounds			
4) N-TETRADECANE	8.041f	200212	1.436 ug/ml
7) N-EICOSANE	12.382	1838915	12.873 ug/ml
10) N-TETRACOSANE	14.606	1387484	9.838 ug/ml
11) N-HEXACOSANE	15.662	240495	1.727 ug/ml
12) N-OCTACOSANE	16.616	655955	4.791 ug/ml
13) N-TRIACONTANE	17.506	528447	3.957 ug/ml
14) N-DOTRIACONTANE	18.333	368579	2.913 ug/ml
15) N-TETRATRIACONTANE	19.127	214122	1.807 ug/ml
16) N-HEXATRIACONTANE	19.857	686890	6.205 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031419\
Data File : FG004185.D
Signal(s) : FID1A.ch
Acq On : 14 Mar 2019 12:00
Operator : AJ\SJ
Sample : K1870-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 14 14:15:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

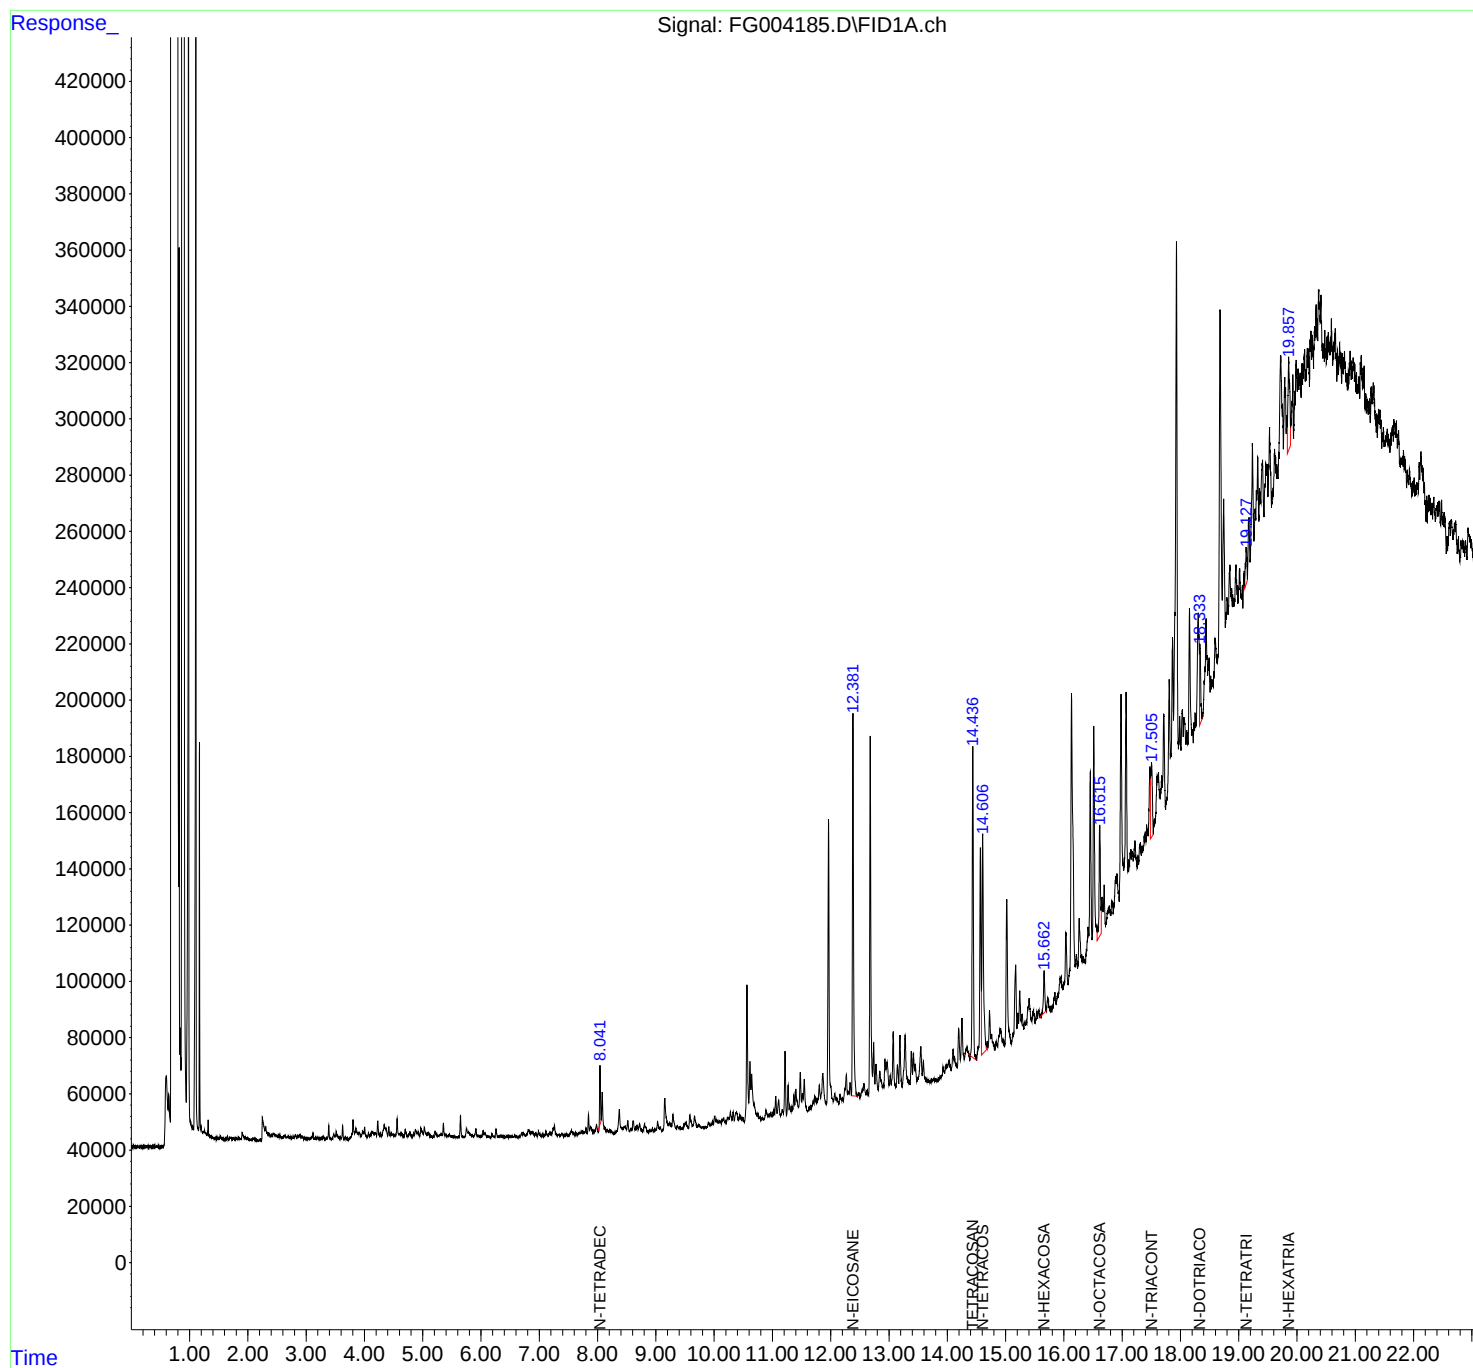


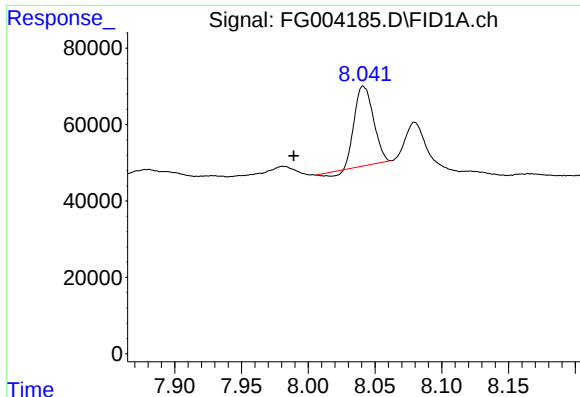

#4 N-TETRADECANE


R.T.: 8.041 min
Delta R.T.: 0.052 min
Response: 200212
Conc: 1.44 ug/ml

Instrument :
FID_G
ClientSampleId :

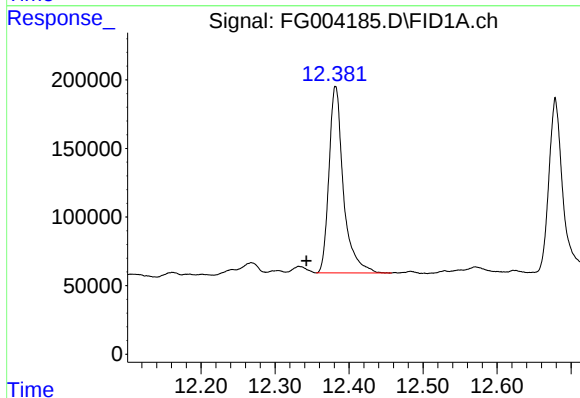


#7 N-EICOSANE

R.T.: 12.382 min
Delta R.T.: 0.039 min
Response: 1838915
Conc: 12.87 ug/ml

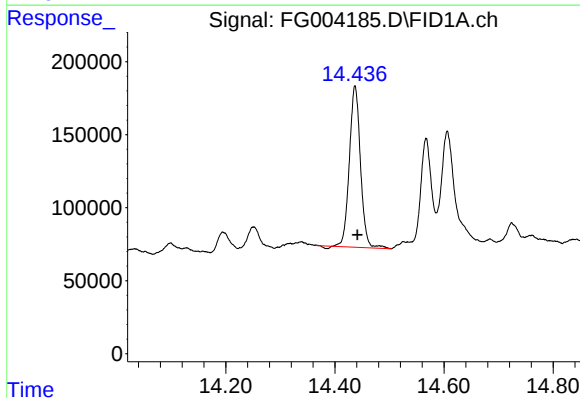


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.437 min
Delta R.T.: -0.004 min
Response: 1556343
Conc: 12.38 ug/ml

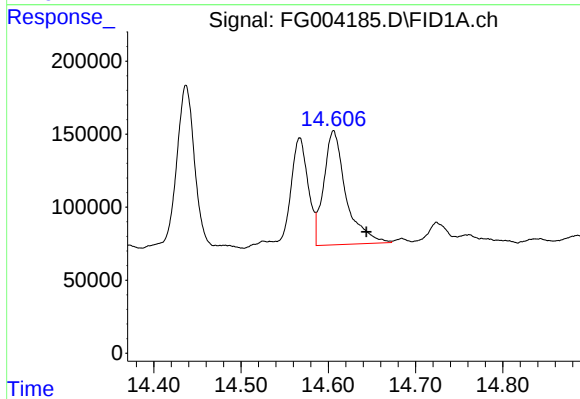

#10 N-TETRACOSANE


R.T.: 14.606 min
Delta R.T.: -0.038 min
Response: 1387484
Conc: 9.84 ug/ml

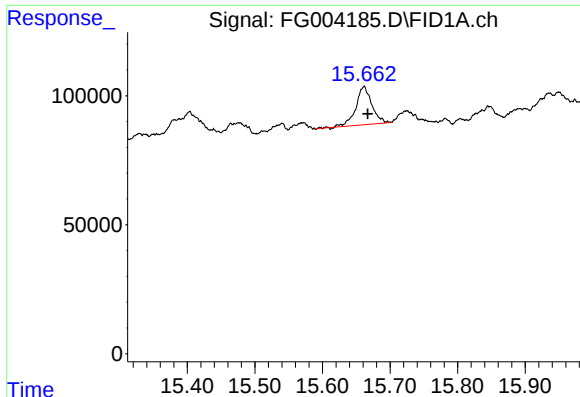

#11 N-HEXACOSANE


R.T.: 15.662 min
Delta R.T.: -0.005 min
Response: 240495
Conc: 1.73 ug/ml

Instrument :
FID_G
ClientSampleId :

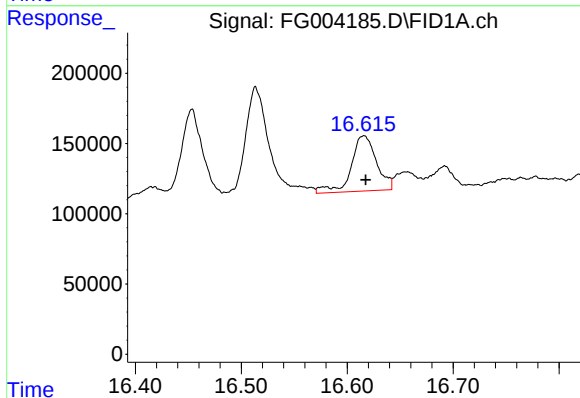


#12 N-OCTACOSANE

R.T.: 16.616 min
Delta R.T.: -0.002 min
Response: 655955
Conc: 4.79 ug/ml

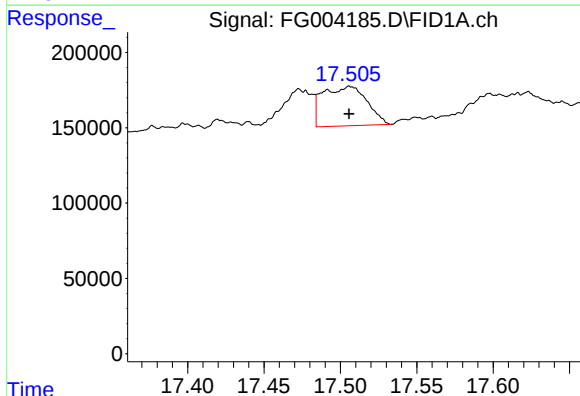


#13 N-TRIACONTANE

R.T.: 17.506 min
Delta R.T.: 0.000 min
Response: 528447
Conc: 3.96 ug/ml

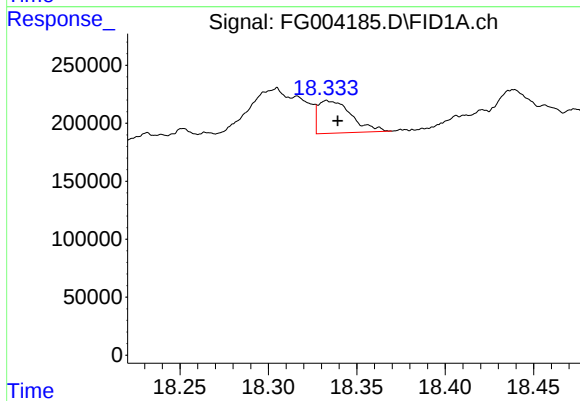

#14 N-DOTRIACONTANE


R.T.: 18.333 min
Delta R.T.: -0.006 min
Response: 368579
Conc: 2.91 ug/ml

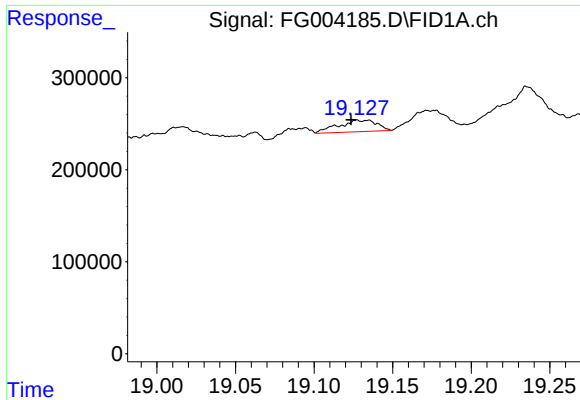

#15 N-TETRATRIACONTANE

R.T.: 19.127 min
Delta R.T.: 0.004 min
Response: 214122
Conc: 1.81 ug/ml

Instrument :
FID_G
ClientSampleId :

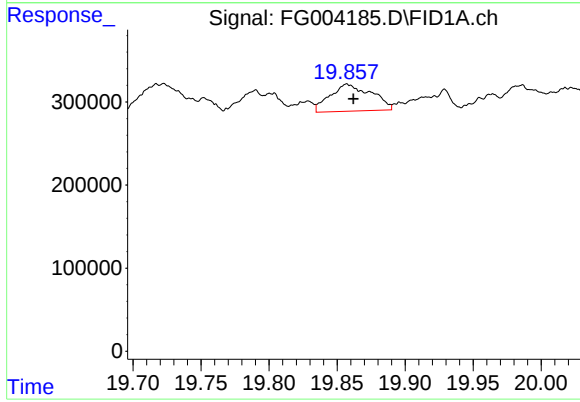

#16 N-HEXATRIACONTANE

R.T.: 19.857 min
Delta R.T.: -0.005 min
Response: 686890
Conc: 6.20 ug/ml