

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031419\
 Data File : FG004187.D
 Signal(s) : FID1A.ch
 Acq On : 14 Mar 2019 13:00
 Operator : AJ\SJ
 Sample : K1870-03 2X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 14 14:15:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
 Quant Title :
 QLast Update : Tue Mar 05 03:05:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.439	618697	4.921 ug/ml
Target Compounds			
7) N-EICOSANE	12.388	390905	2.736 ug/ml
10) N-TETRACOSANE	14.613	371355	2.633 ug/ml
12) N-OCTACOSANE	16.619	177806	1.299 ug/ml
13) N-TRIACONTANE	17.508	589582	4.415 ug/ml
14) N-DOTRIACONTANE	18.342	336024	2.656 ug/ml
15) N-TETRATRIACONTANE	19.130	227568	1.920 ug/ml
16) N-HEXATRIACONTANE	19.871	265449	2.398 ug/ml
17) N-OCTATRIACONTANE	20.586	962522	9.535 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031419\
Data File : FG004187.D
Signal(s) : FID1A.ch
Acq On : 14 Mar 2019 13:00
Operator : AJ\SJ
Sample : K1870-03 2X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 14 14:15:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

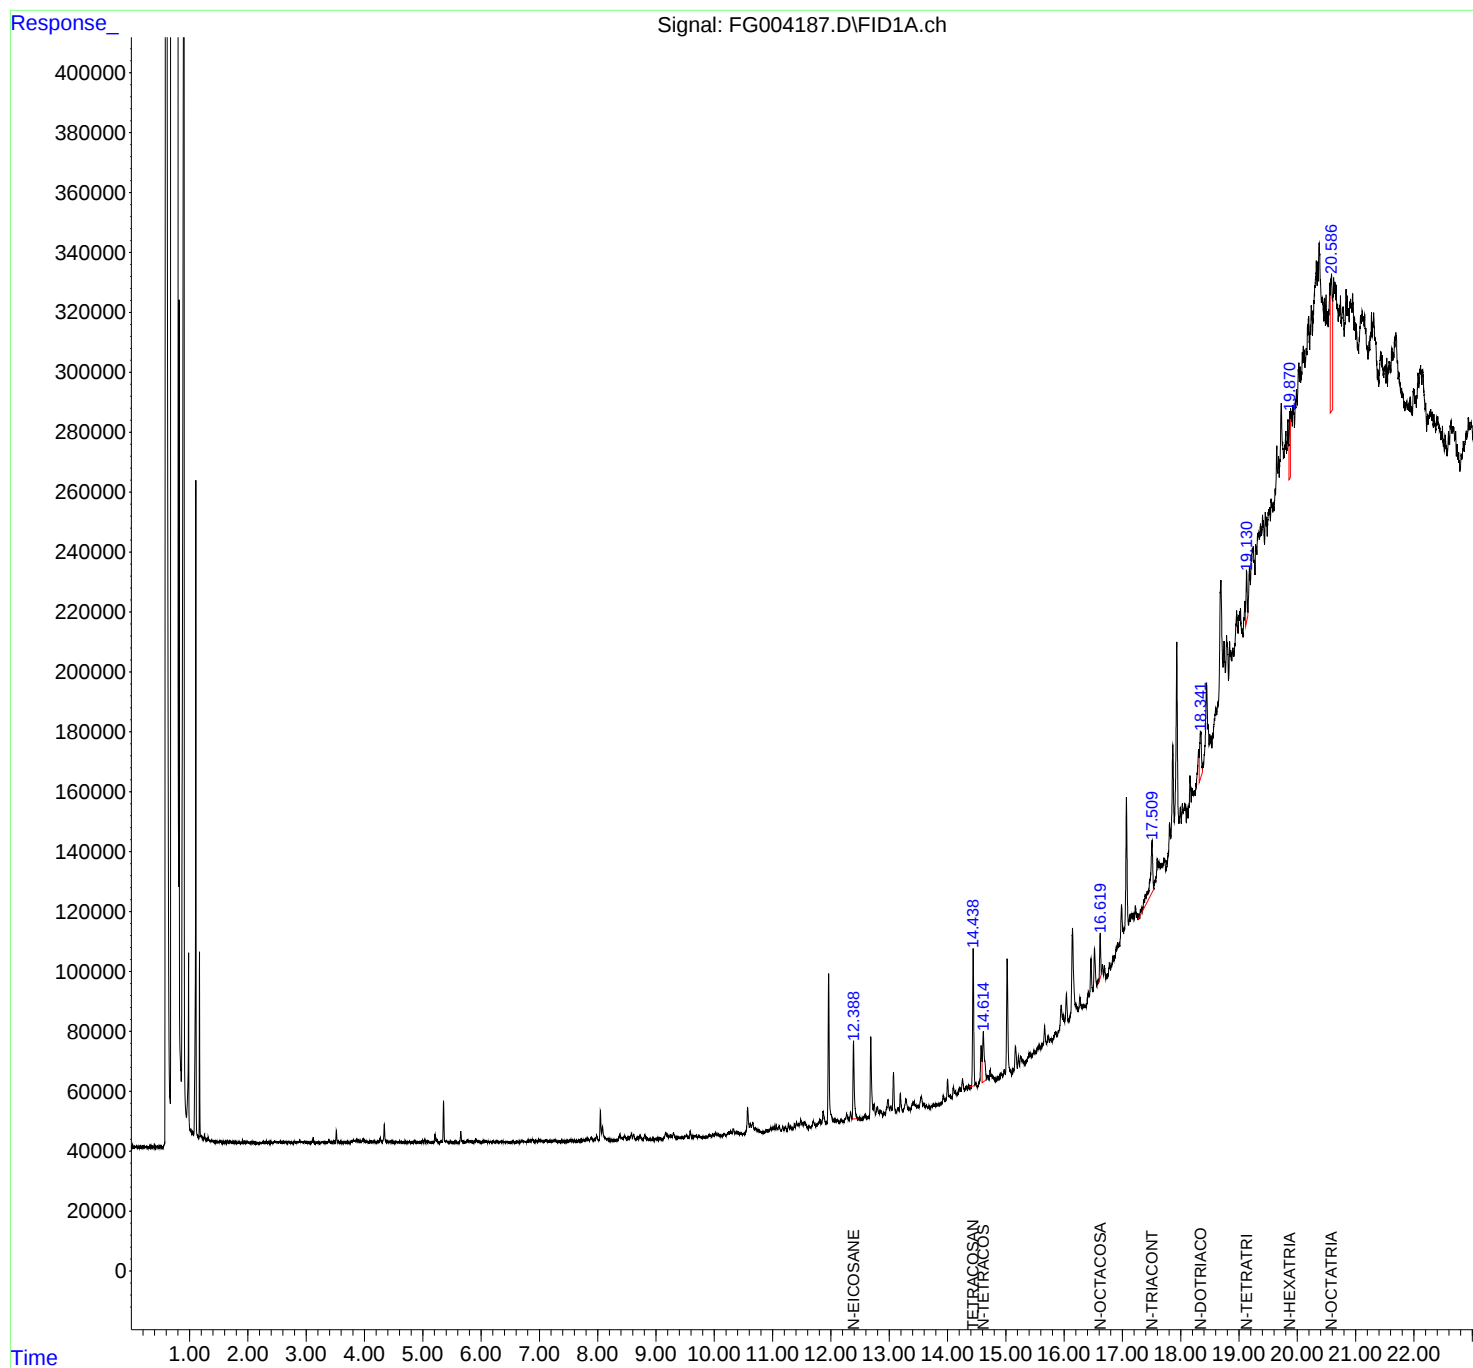


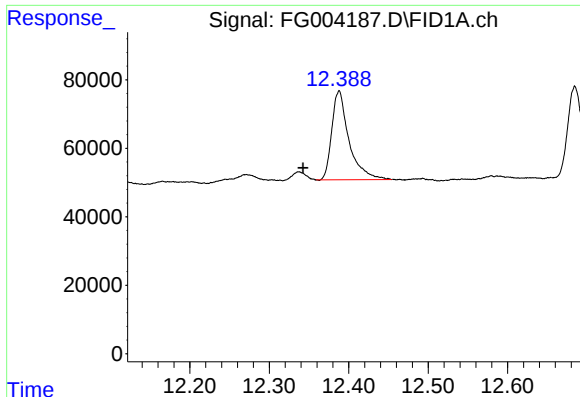

#7 N-EICOSANE


R.T.: 12.388 min
Delta R.T.: 0.045 min
Response: 390905
Conc: 2.74 ug/ml

Instrument :
FID_G
ClientSampleId :

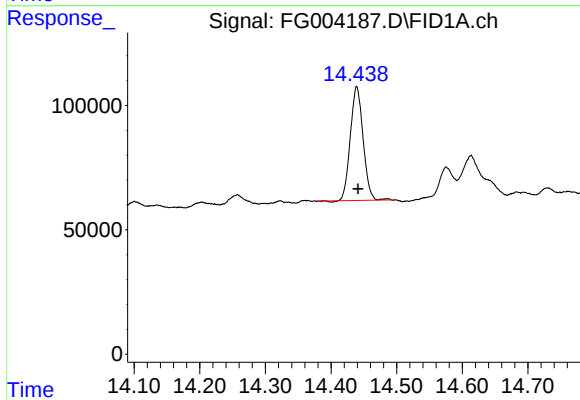


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.439 min
Delta R.T.: -0.002 min
Response: 618697
Conc: 4.92 ug/ml

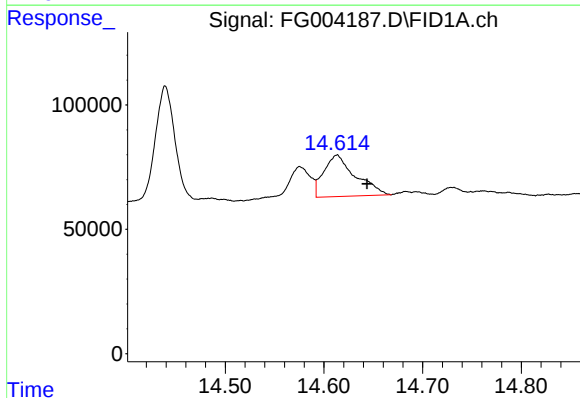


#10 N-TETRACOSANE

R.T.: 14.613 min
Delta R.T.: -0.031 min
Response: 371355
Conc: 2.63 ug/ml

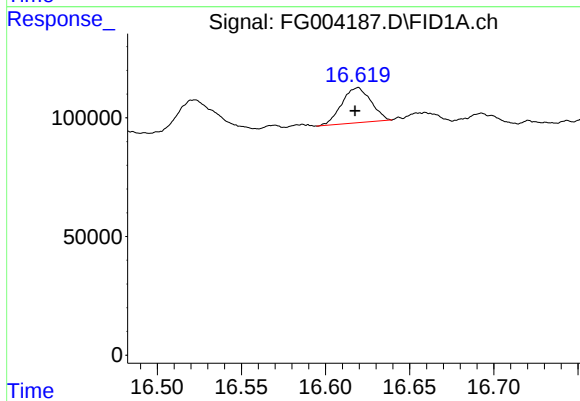

#12 N-OCTACOSANE


R.T.: 16.619 min
Delta R.T.: 0.001 min
Response: 177806
Conc: 1.30 ug/ml

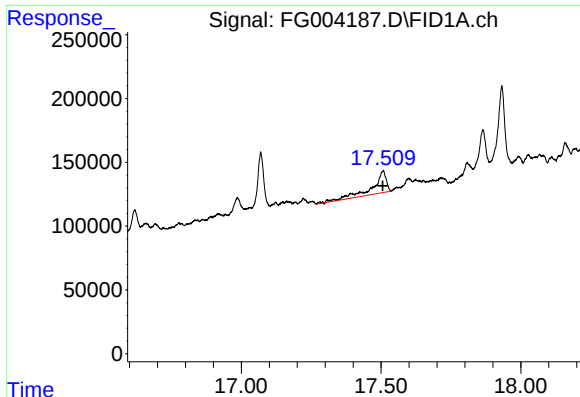

#13 N-TRIACONTANE


R.T.: 17.508 min
Delta R.T.: 0.003 min
Response: 589582
Conc: 4.41 ug/ml

Instrument :
FID_G
ClientSampleId :

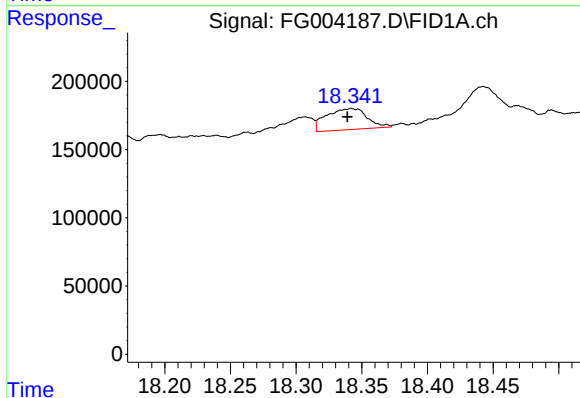


#14 N-DOTRIACONTANE

R.T.: 18.342 min
Delta R.T.: 0.003 min
Response: 336024
Conc: 2.66 ug/ml

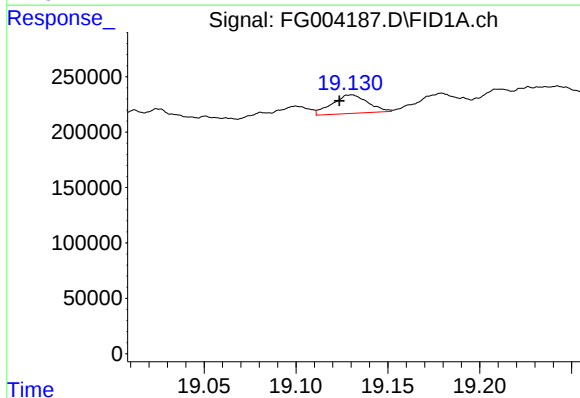


#15 N-TETRATRIACONTANE

R.T.: 19.130 min
Delta R.T.: 0.006 min
Response: 227568
Conc: 1.92 ug/ml

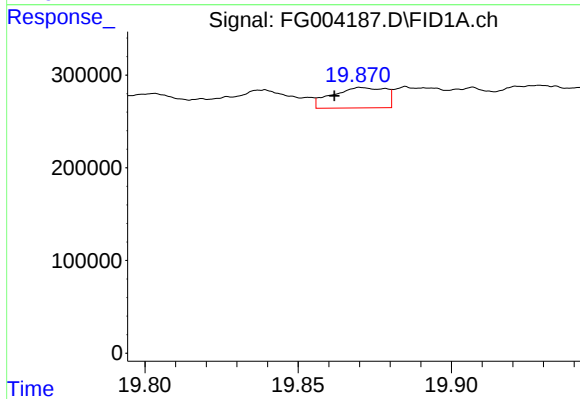

#16 N-HEXATRIACONTANE

R.T.: 19.871 min
Delta R.T.: 0.009 min
Response: 265449
Conc: 2.40 ug/ml

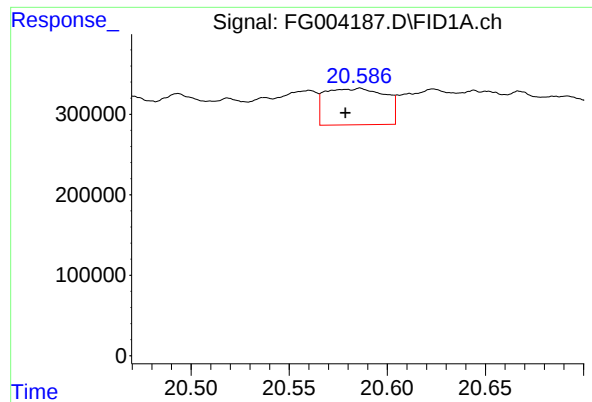

#17 N-OCTATRIACONTANE

R.T.: 20.586 min
Delta R.T.: 0.008 min
Response: 962522
Conc: 9.54 ug/ml

Instrument :
FID_G
ClientSampleId :