

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031419\
 Data File : FG004191.D
 Signal(s) : FID1A.ch
 Acq On : 14 Mar 2019 15:24
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 14 15:46:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
 Quant Title :
 QLast Update : Tue Mar 05 03:05:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.445	2206223	17.549 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.510	210956	1.580 ug/ml
15) N-TETRATRIACONTANE	19.129	333220	2.812 ug/ml
16) N-HEXATRIACONTANE	19.883	171138	1.546 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031419\
Data File : FG004191.D
Signal(s) : FID1A.ch
Acq On : 14 Mar 2019 15:24
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 14 15:46:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

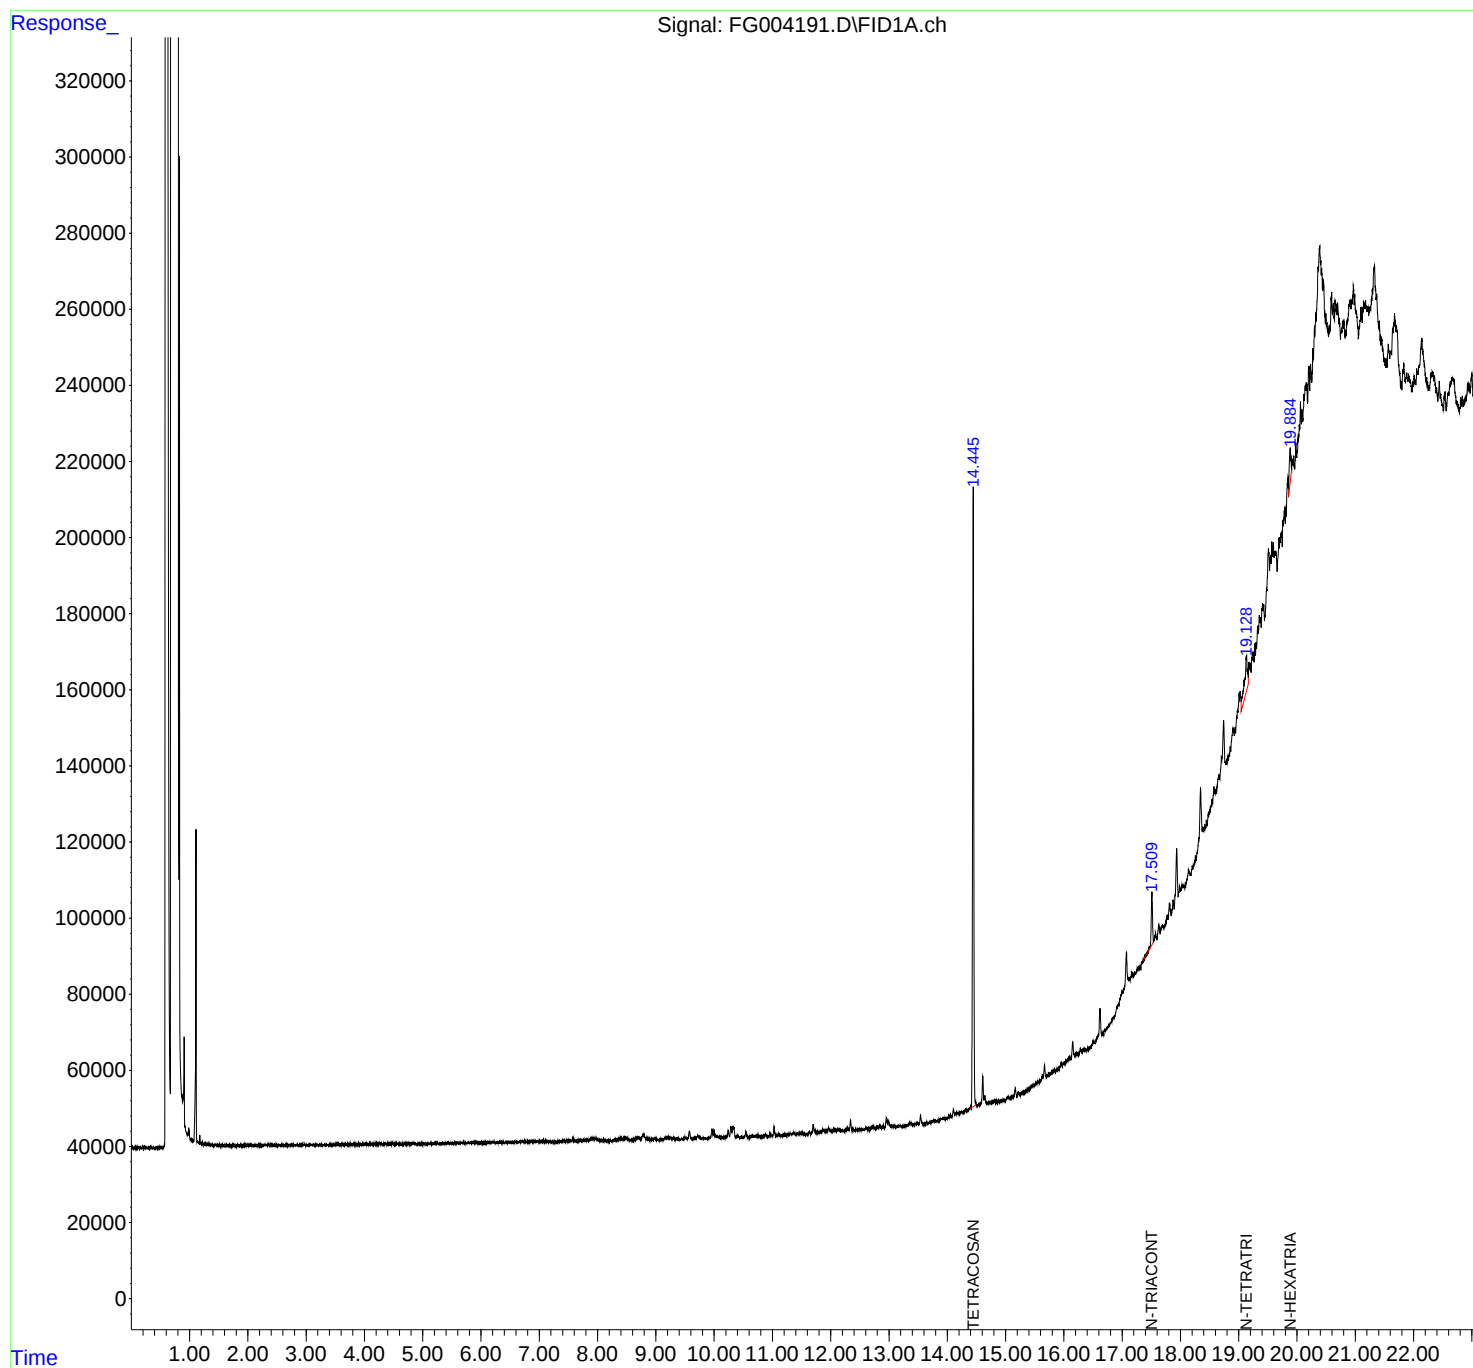


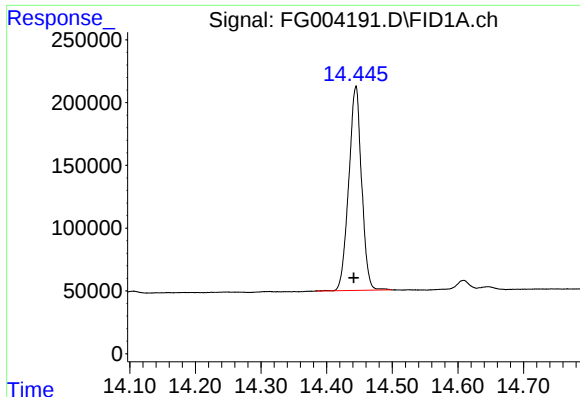

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.445 min
Delta R.T.: 0.003 min
Response: 2206223
Conc: 17.55 ug/ml

Instrument :
FID_G
ClientSampleId :

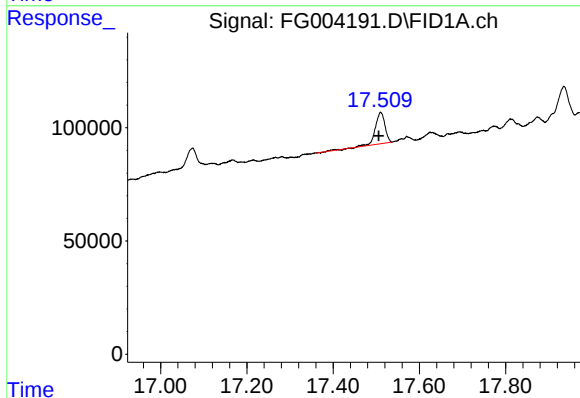


#13 N-TRIACONTANE

R.T.: 17.510 min
Delta R.T.: 0.005 min
Response: 210956
Conc: 1.58 ug/ml

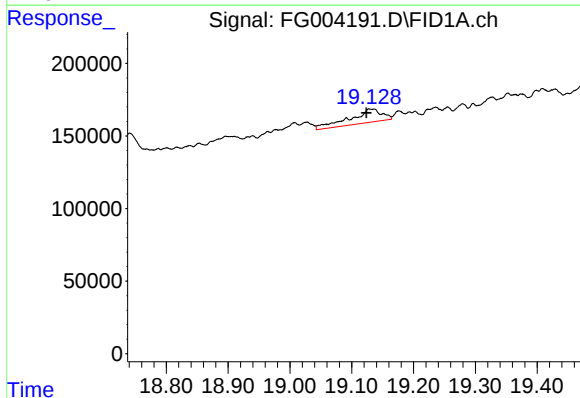

#15 N-TETRATRIACONTANE

R.T.: 19.129 min
Delta R.T.: 0.005 min
Response: 333220
Conc: 2.81 ug/ml

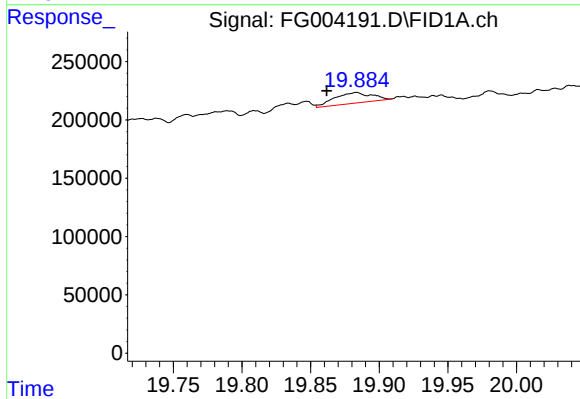

#16 N-HEXATRIACONTANE

R.T.: 19.883 min
Delta R.T.: 0.022 min
Response: 171138
Conc: 1.55 ug/ml