

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031419\
Data File : FG004183.D
Signal(s) : FID1A.ch
Acq On : 14 Mar 2019 10:59
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 14 14:15:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.188	3361642	24.797 ug/ml
12)	N-OCTACOSANE	16.612	3277901	23.942 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031419\
Data File : FG004183.D
Signal(s) : FID1A.ch
Acq On : 14 Mar 2019 10:59
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 14 14:15:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

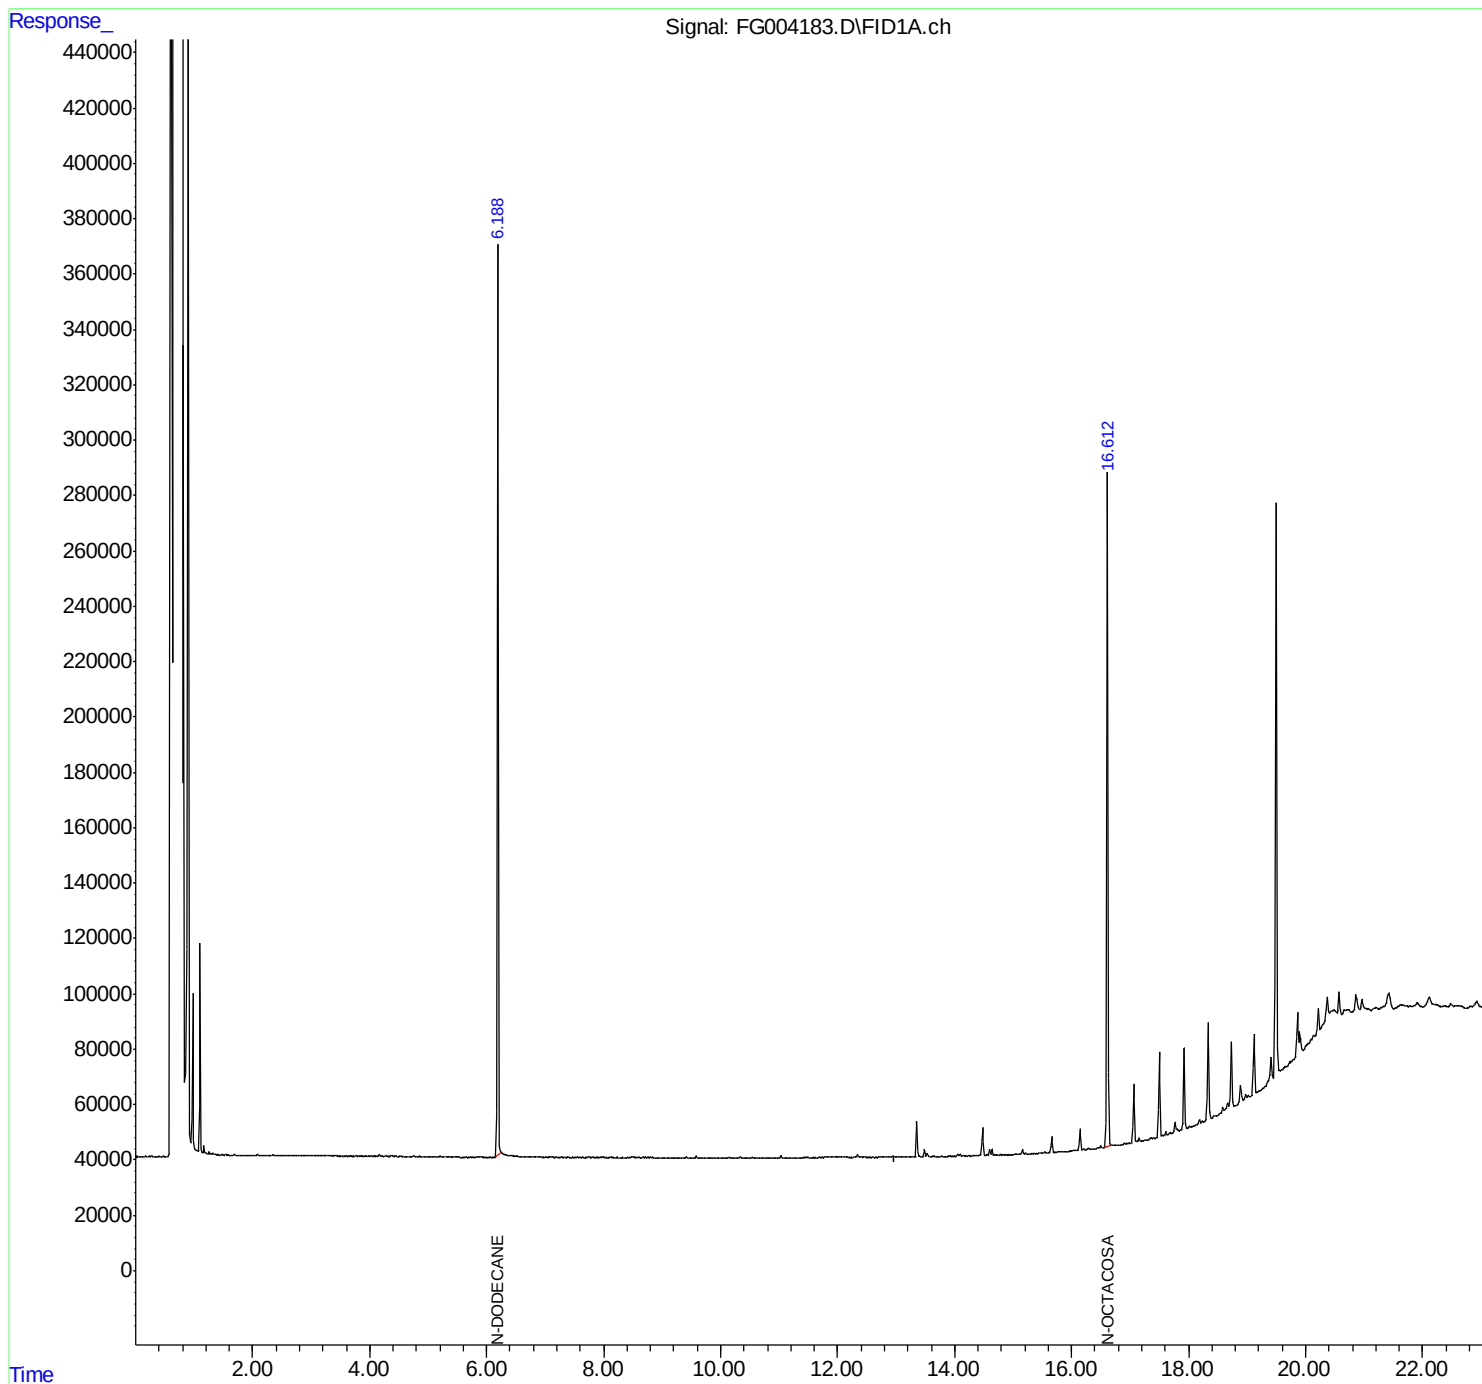


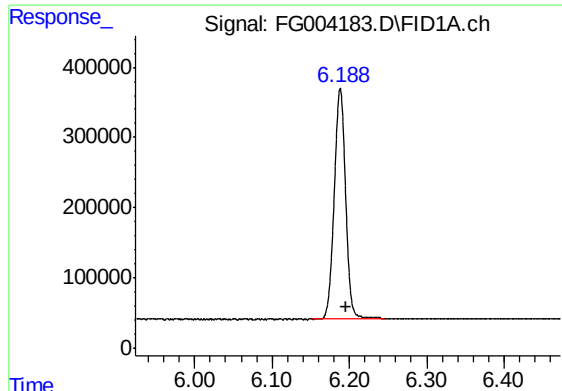

#3 N-DODECANE


R.T.: 6.188 min
Delta R.T.: -0.007 min
Response: 3361642
Conc: 24.80 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

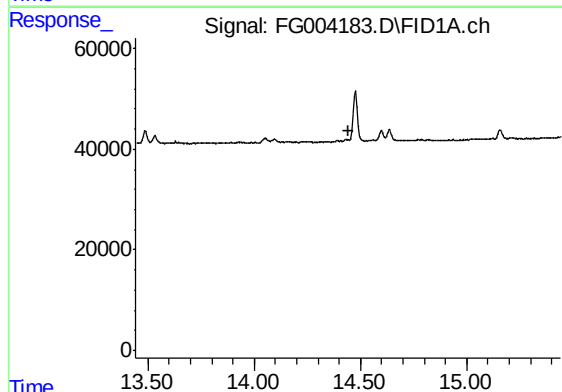

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.441 min
Response: 0
Conc: N.D.

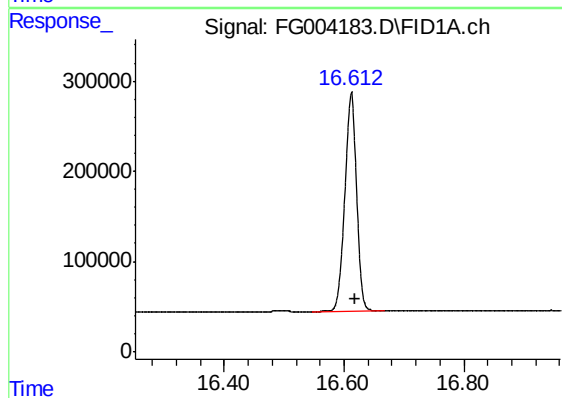

#12 N-OCTACOSANE

R.T.: 16.612 min
Delta R.T.: -0.005 min
Response: 3277901
Conc: 23.94 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

rteres

Area Percent Report

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031419\
Data File : FG004183.D
Signal(s) : FID1A.ch
Acq On : 14 Mar 2019 10:59
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Title :

Signal : FID1A.ch

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	6.188	6.152	6.244	BB	329922	3361642	100.00%	50.631%
2	16.612	16.547	16.666	BB	242991	3277901	97.51%	49.369%
Sum of corrected areas:							6639543	

FG030419.M Thu Mar 14 14:18:46 2019