

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031423\
 Data File : FG011592.D
 Signal(s) : FID1A.ch
 Acq On : 14 Mar 2023 20:15
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: Mar 15 05:11:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG022123.M
 Quant Title :
 QLast Update : Tue Feb 21 16:44:49 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.058	5433629	51.660 ug/ml
Target Compounds			
2) N-DECANE	4.581	6221533	51.070 ug/ml
3) N-DODECANE	6.752	6346724	51.328 ug/ml
4) N-TETRADECANE	8.582	6369289	51.548 ug/ml
5) N-HEXADECANE	10.195	6475520	51.324 ug/ml
6) N-OCTADECANE	11.641	6476367	51.300 ug/ml
7) N-EICOSANE	12.955	6420415	51.293 ug/ml
8) N-DOCOSANE	14.156	6176154	51.477 ug/ml
10) N-TETRACOSANE	15.263	6085939	51.576 ug/ml
11) N-HEXACOSANE	16.286	5858840	51.471 ug/ml
12) N-OCTACOSANE	17.238	5637951	51.380 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031423\
Data File : FG011592.D
Signal(s) : FID1A.ch
Acq On : 14 Mar 2023 20:15
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: Mar 15 05:11:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG022123.M
Quant Title :
QLast Update : Tue Feb 21 16:44:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

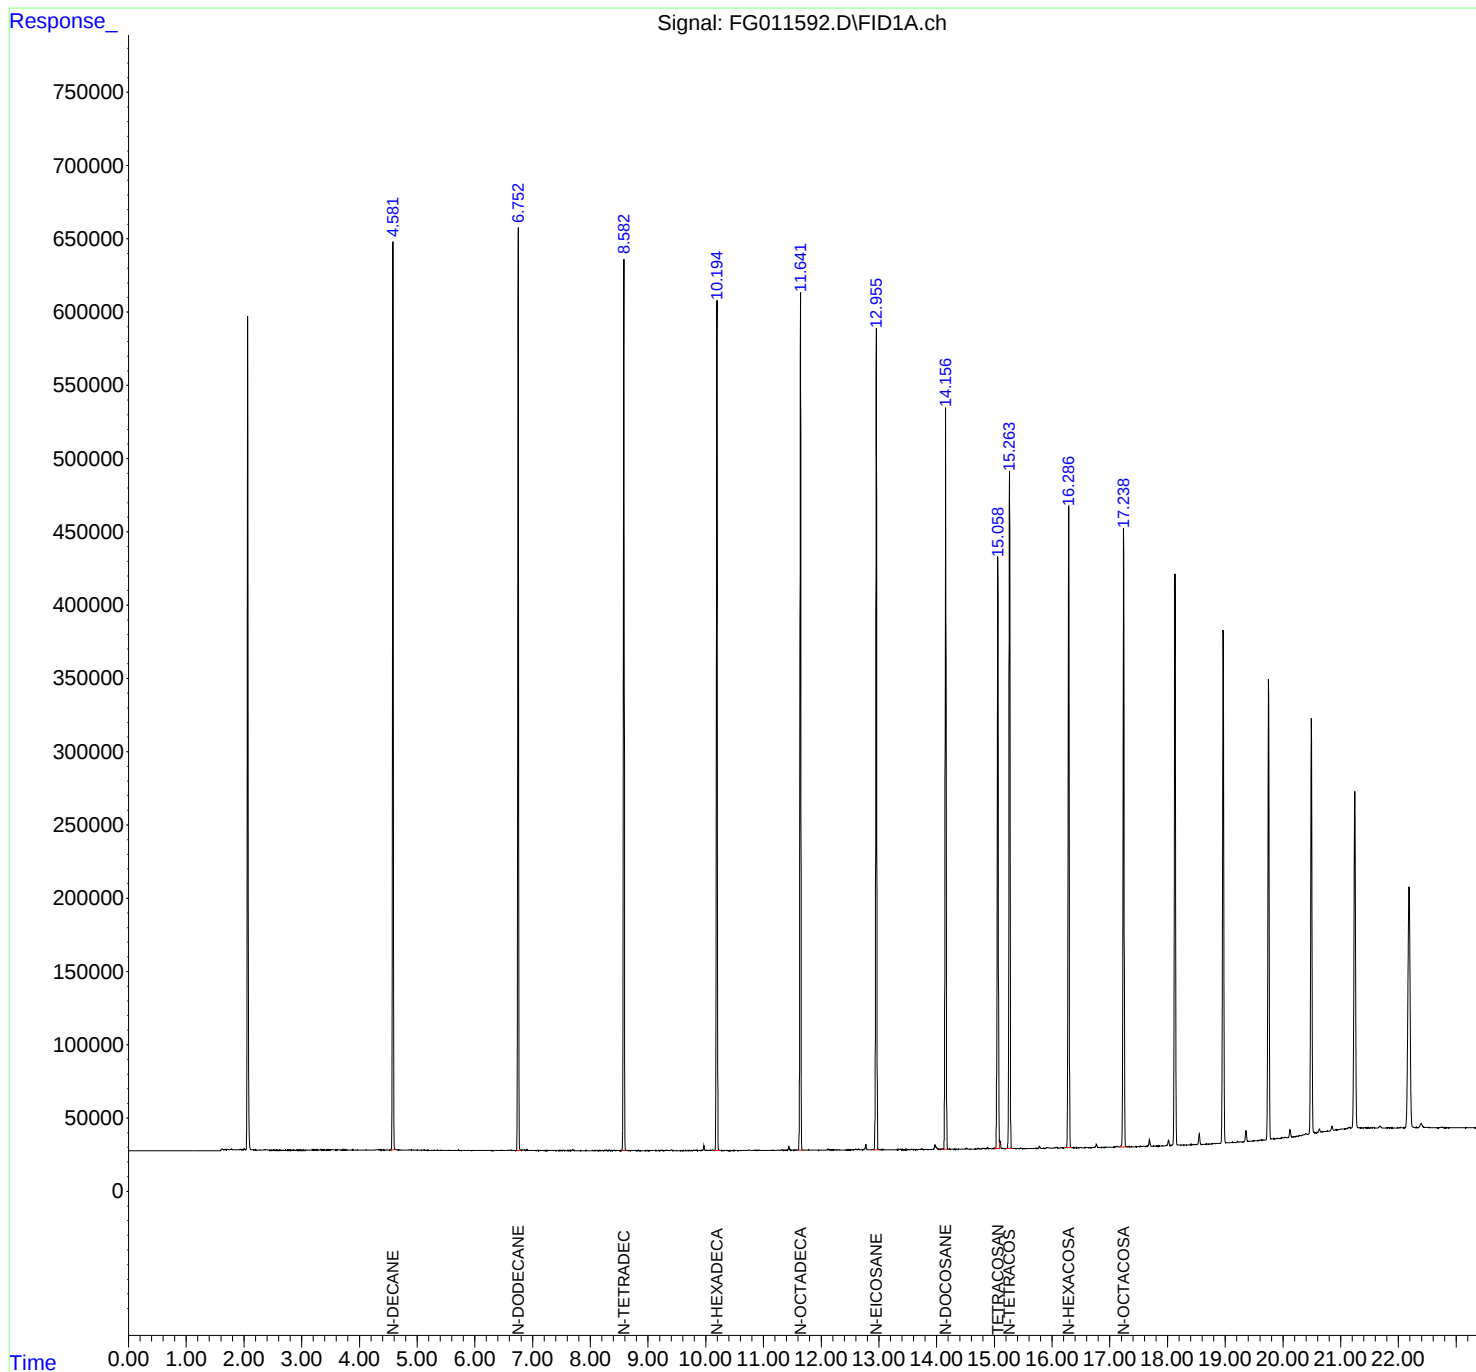


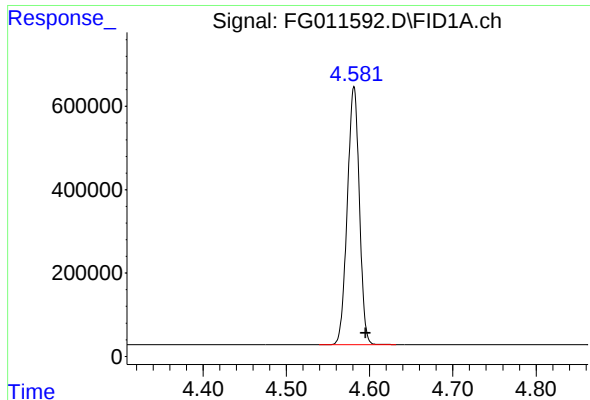

#2 N-DECANE


R.T.: 4.581 min
Delta R.T.: -0.014 min
Response: 6221533
Conc: 51.07 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

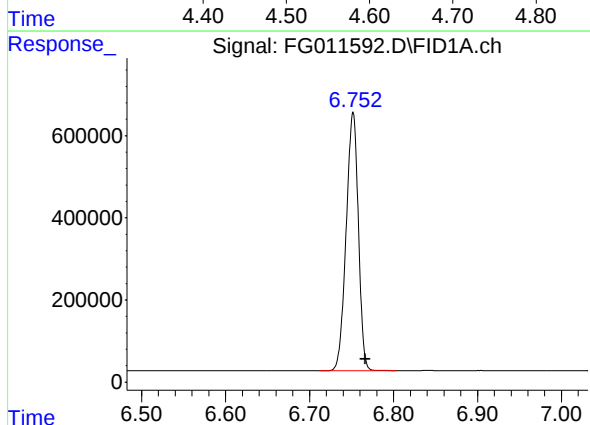


#3 N-DODECANE

R.T.: 6.752 min
Delta R.T.: -0.014 min
Response: 6346724
Conc: 51.33 ug/ml

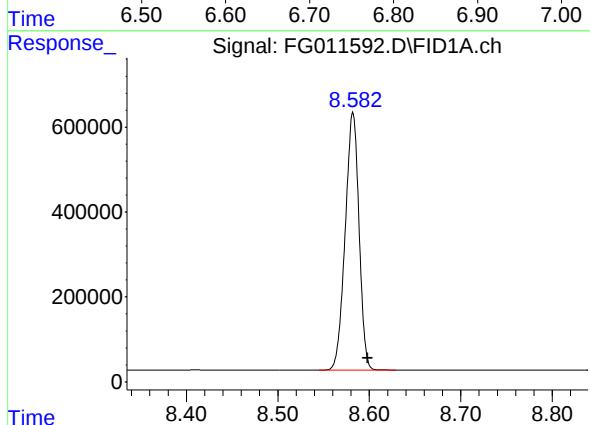


#4 N-TETRADECANE

R.T.: 8.582 min
Delta R.T.: -0.016 min
Response: 6369289
Conc: 51.55 ug/ml

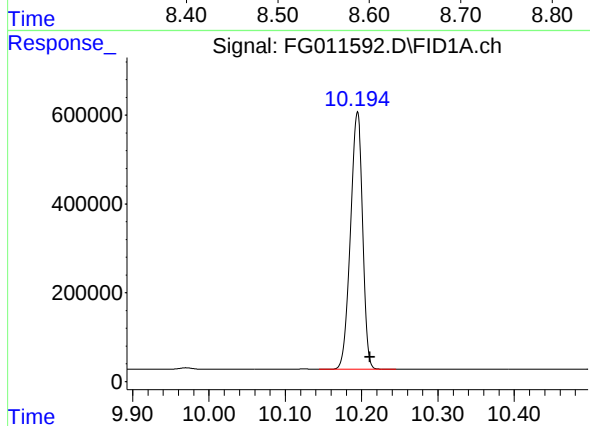

#5 N-HEXADECANE


R.T.: 10.195 min
Delta R.T.: -0.016 min
Response: 6475520
Conc: 51.32 ug/ml

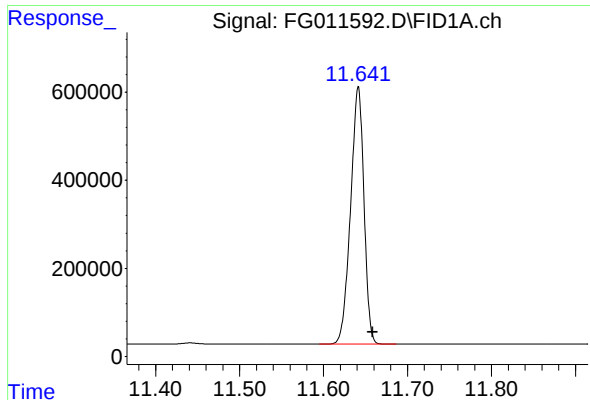

#6 N-OCTADECANE


R.T.: 11.641 min
Delta R.T.: -0.017 min
Response: 6476367
Conc: 51.30 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

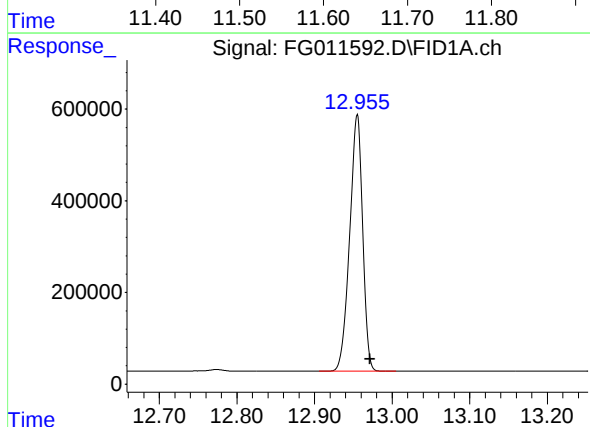


#7 N-EICOSANE

R.T.: 12.955 min
Delta R.T.: -0.016 min
Response: 6420415
Conc: 51.29 ug/ml

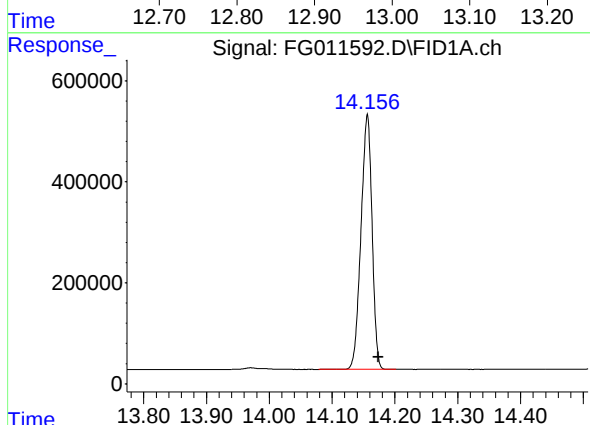


#8 N-DOCOSANE

R.T.: 14.156 min
Delta R.T.: -0.018 min
Response: 6176154
Conc: 51.48 ug/ml

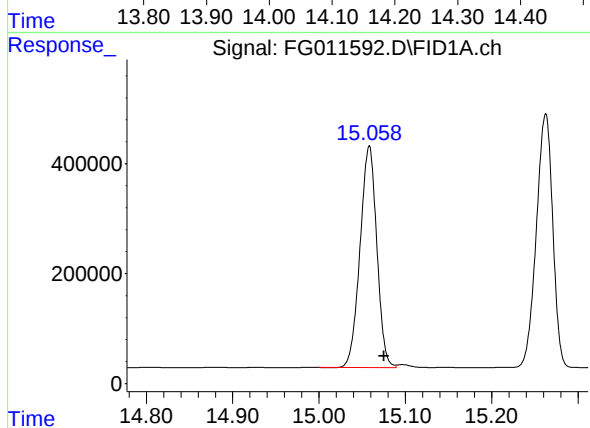

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.058 min
Delta R.T.: -0.017 min
Response: 5433629
Conc: 51.66 ug/ml

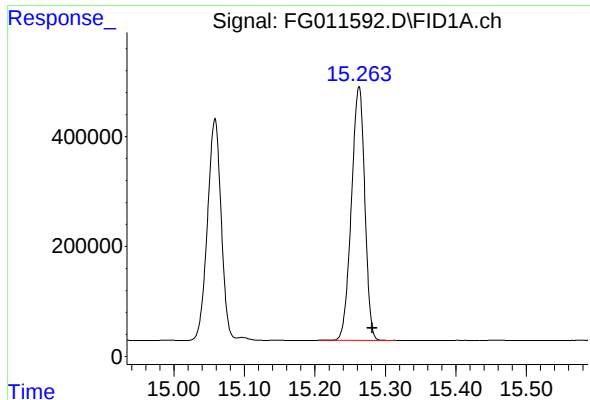

#10 N-TETRACOSANE


R.T.: 15.263 min
Delta R.T.: -0.018 min
Response: 6085939
Conc: 51.58 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

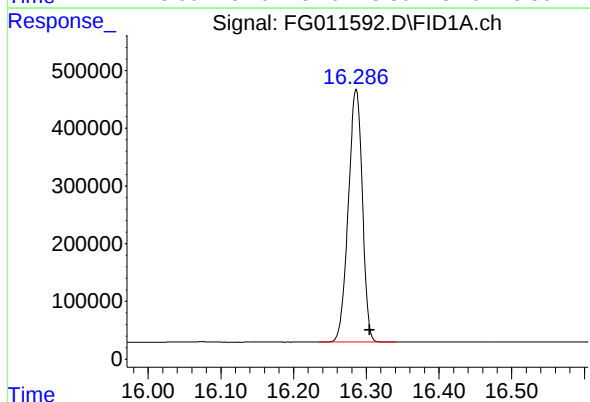

#11 N-HEXACOSANE

R.T.: 16.286 min
Delta R.T.: -0.019 min
Response: 5858840
Conc: 51.47 ug/ml

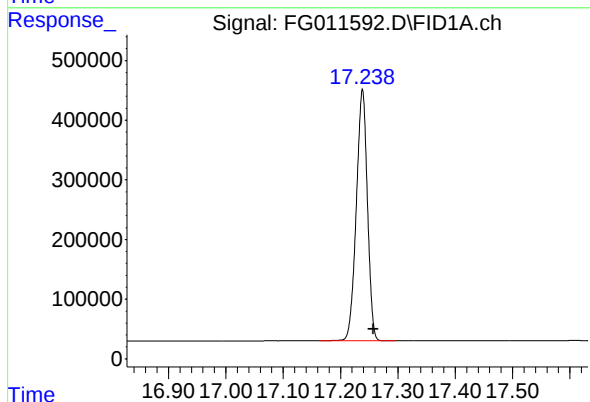

#12 N-OCTACOSANE

R.T.: 17.238 min
Delta R.T.: -0.019 min
Response: 5637951
Conc: 51.38 ug/ml