

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031424\
Data File : FG013646.D
Signal(s) : FID1A.ch
Acq On : 14 Mar 2024 20:55
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 15 01:38:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG022824.M
Quant Title :
QLast Update : Wed Feb 28 13:13:27 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.068	1996795	16.871 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.975	69713	0.597 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031424\
Data File : FG013646.D
Signal(s) : FID1A.ch
Acq On : 14 Mar 2024 20:55
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 15 01:38:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG022824.M
Quant Title :
QLast Update : Wed Feb 28 13:13:27 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

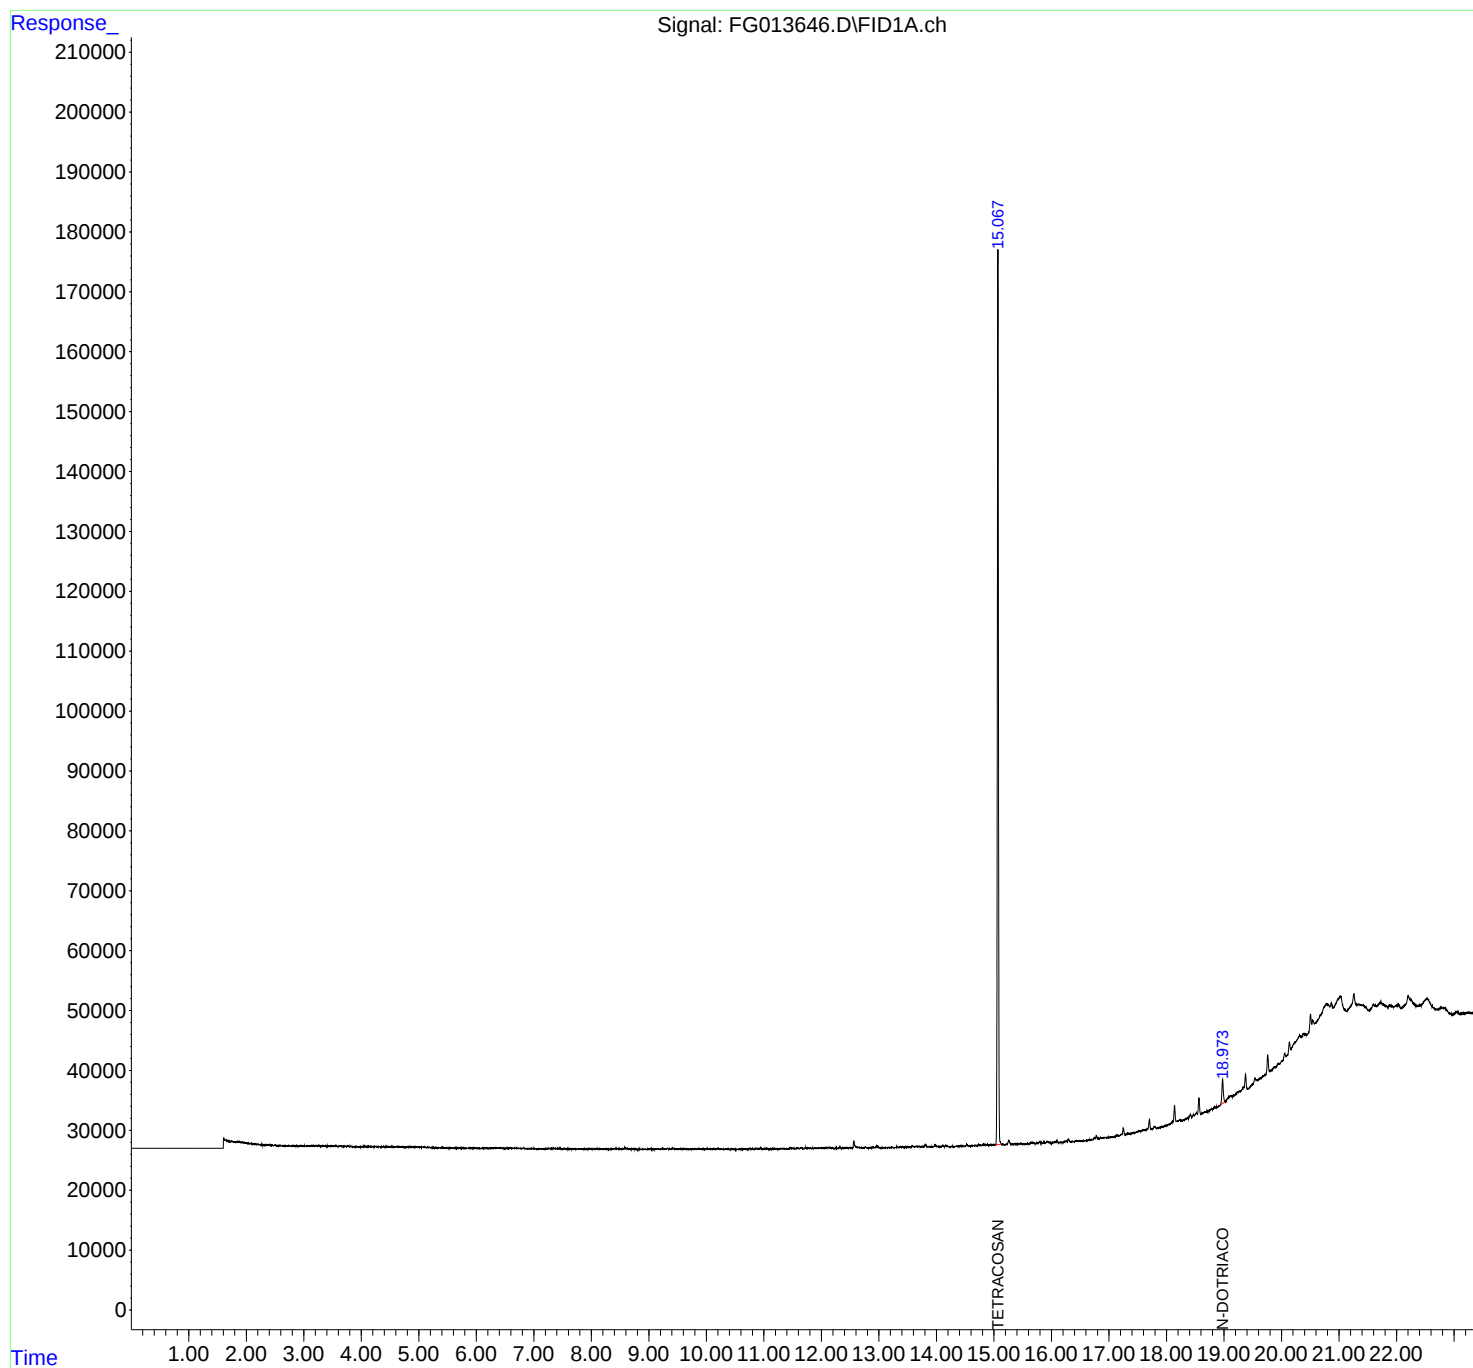

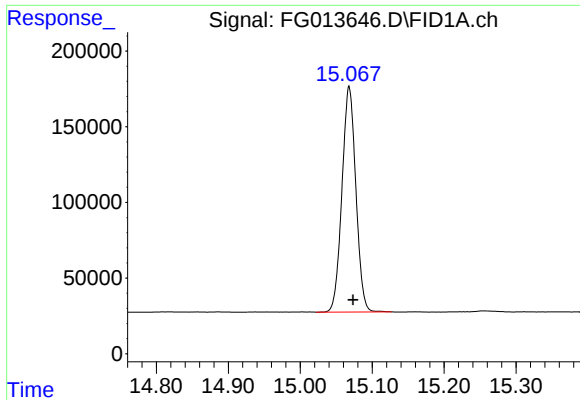

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.068 min
Delta R.T.: -0.005 min
Response: 1996795
Conc: 16.87 ug/ml

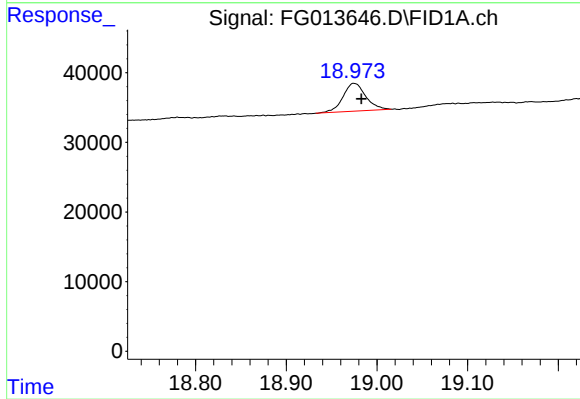

#14 N-DOTRIACONTANE

R.T.: 18.975 min
Delta R.T.: -0.008 min
Response: 69713
Conc: 0.60 ug/ml