

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031424\
 Data File : FG013628.D
 Signal(s) : FID1A.ch
 Acq On : 14 Mar 2024 10:36
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 15 01:34:49 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG022824.M
 Quant Title :
 QLast Update : Wed Feb 28 13:13:27 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.071	5955646	50.320 ug/ml
Target Compounds			
2) N-DECANE	4.583	6685542	52.165 ug/ml
3) N-DODECANE	6.756	6893257	51.670 ug/ml
4) N-TETRADECANE	8.589	6724918	51.501 ug/ml
5) N-HEXADECANE	10.202	6803468	51.202 ug/ml
6) N-OCTADECANE	11.650	6962630	50.883 ug/ml
7) N-EICOSANE	12.965	6734941	50.524 ug/ml
8) N-DOCOSANE	14.169	6578565	50.341 ug/ml
10) N-TETRACOSANE	15.276	6474138	50.169 ug/ml
11) N-HEXACOSANE	16.300	6322341	50.207 ug/ml
12) N-OCTACOSANE	17.254	6222201	50.339 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031424\
Data File : FG013628.D
Signal(s) : FID1A.ch
Acq On : 14 Mar 2024 10:36
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 15 01:34:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG022824.M
Quant Title :
QLast Update : Wed Feb 28 13:13:27 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

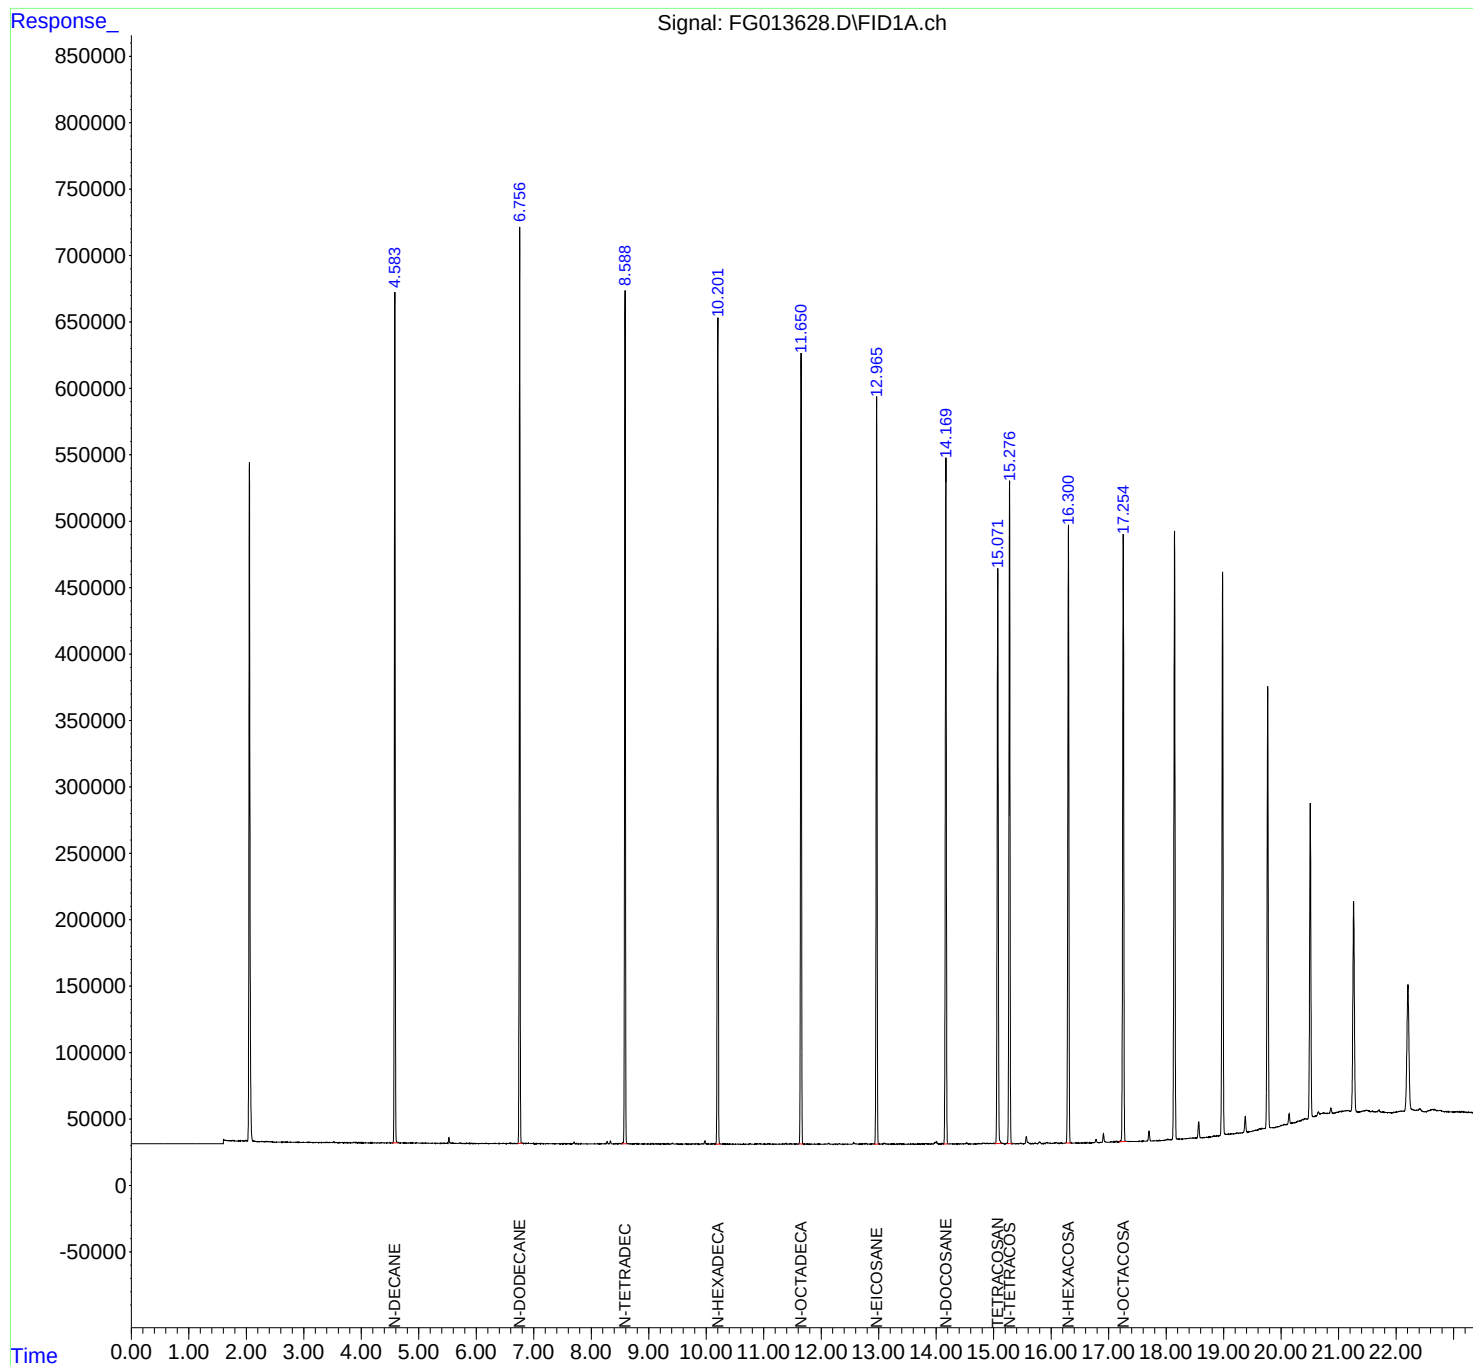

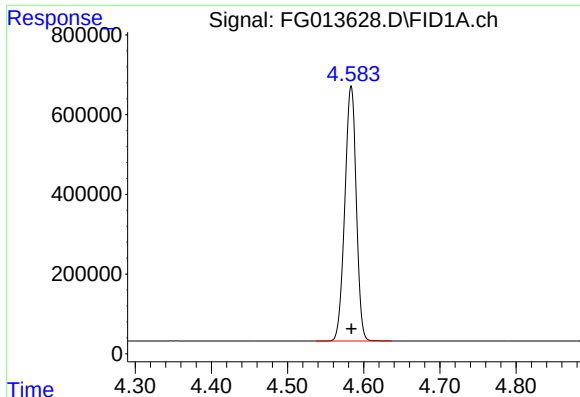


#2 N-DECANE

R.T.: 4.583 min
Delta R.T.: 0.000 min
Response: 6685542
Conc: 52.16 ug/ml

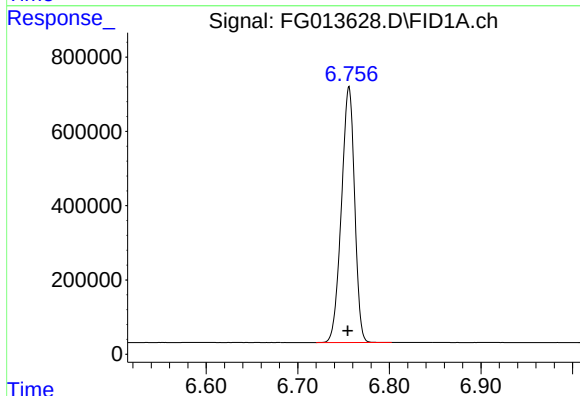


#3 N-DODECANE

R.T.: 6.756 min
Delta R.T.: 0.001 min
Response: 6893257
Conc: 51.67 ug/ml

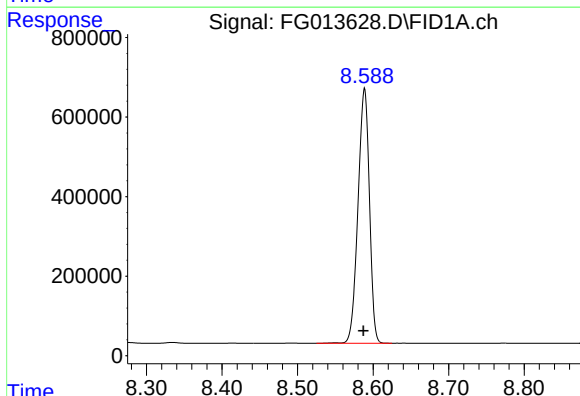


#4 N-TETRADECANE

R.T.: 8.589 min
Delta R.T.: 0.001 min
Response: 6724918
Conc: 51.50 ug/ml

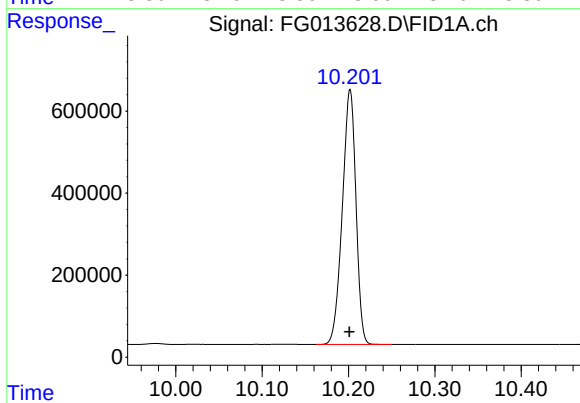


#5 N-HEXADECANE

R.T.: 10.202 min
Delta R.T.: 0.000 min
Response: 6803468
Conc: 51.20 ug/ml

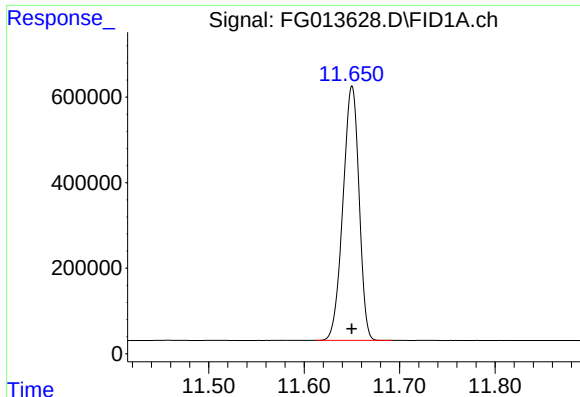


#6 N-OCTADECANE

R.T.: 11.650 min
Delta R.T.: 0.000 min
Response: 6962630
Conc: 50.88 ug/ml

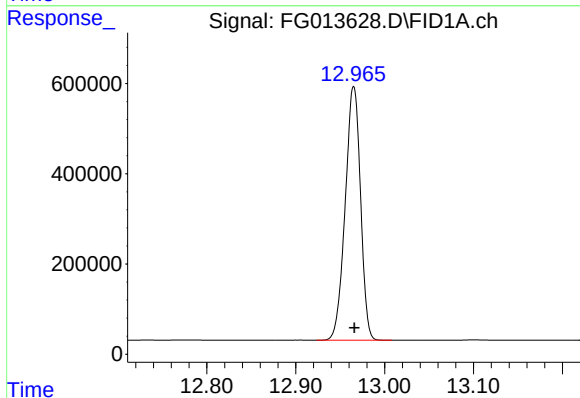


#7 N-EICOSANE

R.T.: 12.965 min
Delta R.T.: 0.000 min
Response: 6734941
Conc: 50.52 ug/ml

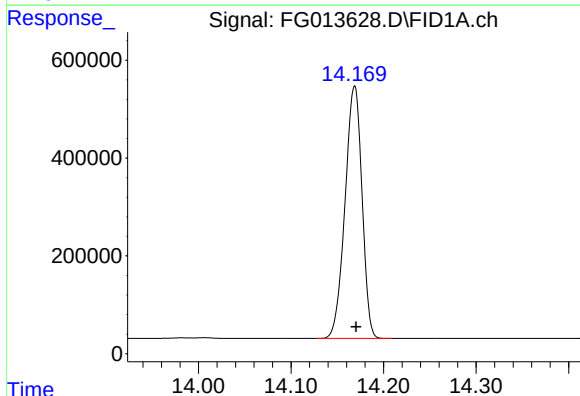


#8 N-DOCOSANE

R.T.: 14.169 min
Delta R.T.: -0.001 min
Response: 6578565
Conc: 50.34 ug/ml

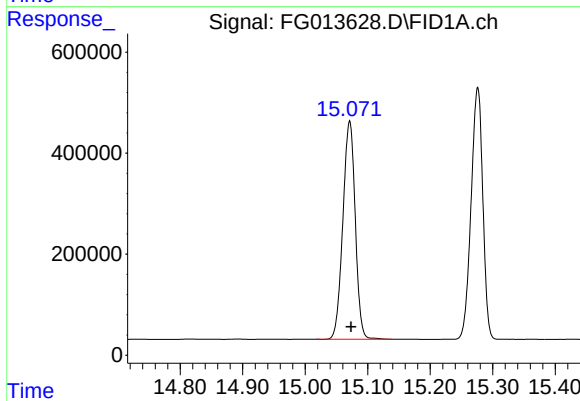


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.071 min
Delta R.T.: -0.002 min
Response: 5955646
Conc: 50.32 ug/ml

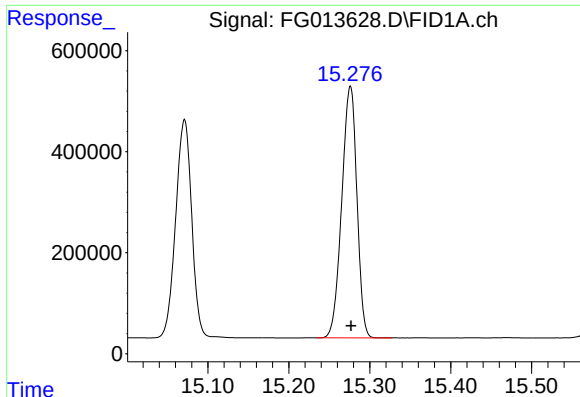


#10 N-TETRACOSANE

R.T.: 15.276 min
Delta R.T.: 0.000 min
Response: 6474138
Conc: 50.17 ug/ml

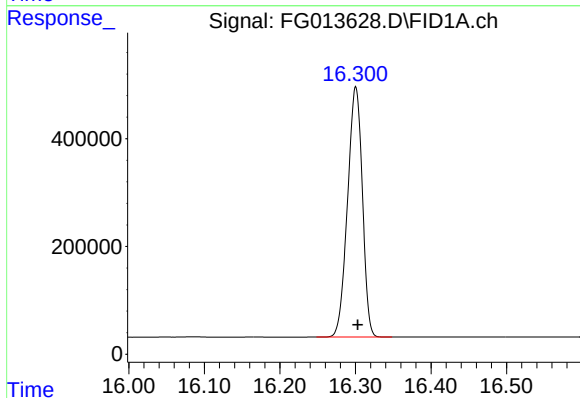

#11 N-HEXACOSANE

R.T.: 16.300 min
Delta R.T.: -0.002 min
Response: 6322341
Conc: 50.21 ug/ml

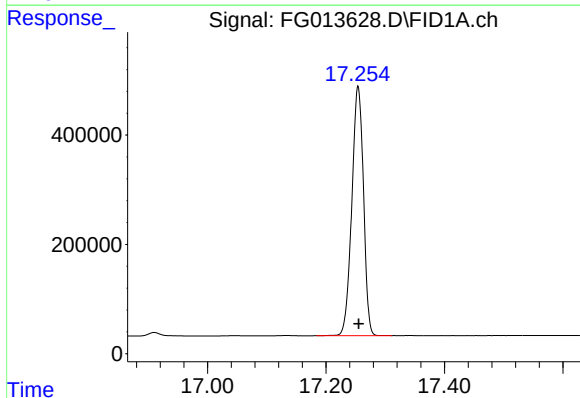

#12 N-OCTACOSANE

R.T.: 17.254 min
Delta R.T.: -0.001 min
Response: 6222201
Conc: 50.34 ug/ml