

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031521\
Data File : FG007700.D
Signal(s) : FID1A.ch
Acq On : 15 Mar 2021 11:36
Operator : DD\AJ
Sample : PB135098BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB135098BL

Integration File: autoint1.e
Quant Time: Mar 15 12:02:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031221.M
Quant Title :
QLast Update : Mon Mar 15 09:29:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.449	2306300	18.227 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031521\
Data File : FG007700.D
Signal(s) : FID1A.ch
Acq On : 15 Mar 2021 11:36
Operator : DD\AJ
Sample : PB135098BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB135098BL

Integration File: autoint1.e
Quant Time: Mar 15 12:02:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031221.M
Quant Title :
QLast Update : Mon Mar 15 09:29:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

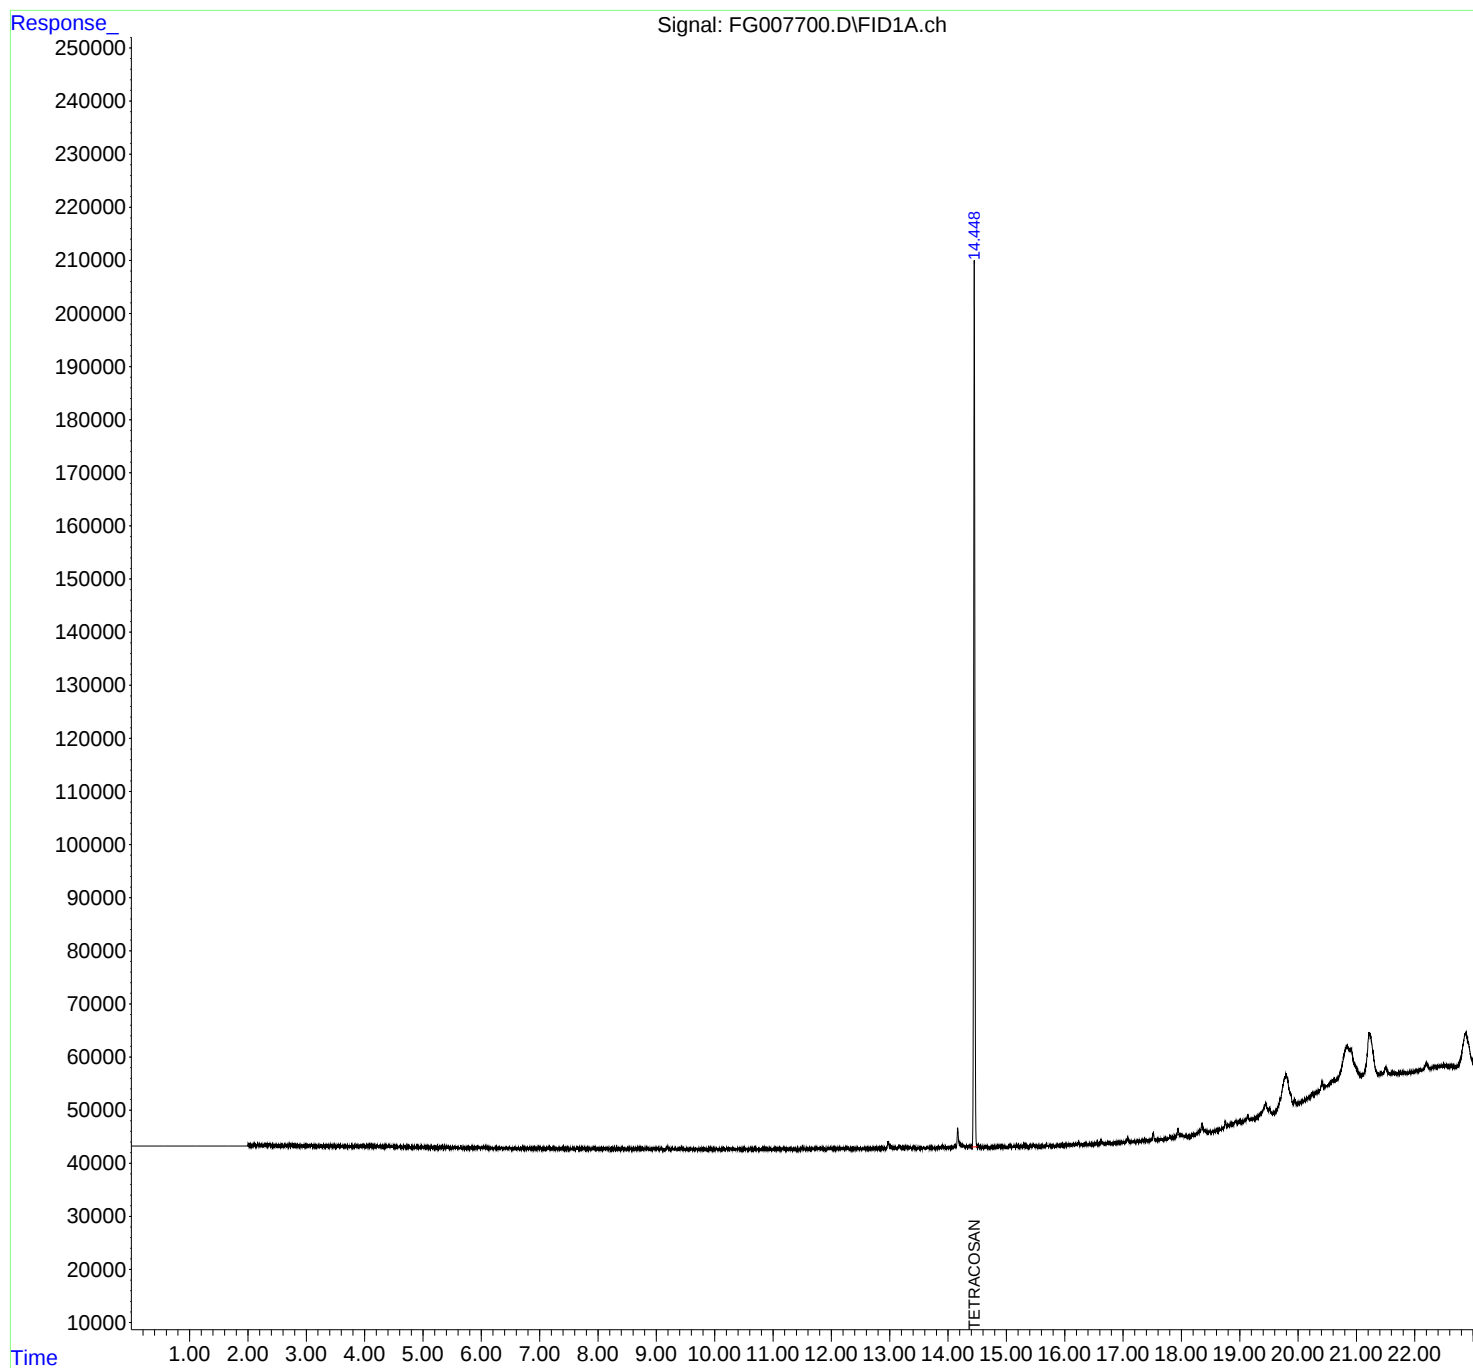

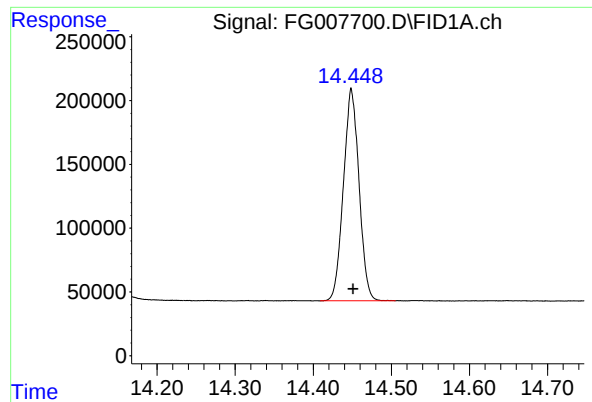

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.449 min
Delta R.T.: -0.002 min
Response: 2306300
Conc: 18.23 ug/ml

Instrument :
FID_G
ClientSampleId :
PB135098BL