

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031619\
 Data File : FG004215.D
 Signal(s) : FID1A.ch
 Acq On : 15 Mar 2019 14:19
 Operator : AJ\SJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Mar 15 23:54:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
 Quant Title :
 QLast Update : Tue Mar 05 03:05:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds				
3) N-DODECANE	6.188	4192651	30.927	ug/ml
12) N-OCTACOSANE	16.612	3861165	28.202	ug/ml
13) N-TRIACONTANE	17.500	563645	4.221	ug/ml
14) N-DOTRIACONTANE	18.333	642221	5.076	ug/ml
15) N-TETRATRIACONTANE	19.120	446190	3.765	ug/ml
16) N-HEXATRIACONTANE	19.862	207720	1.876	ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031619\
Data File : FG004215.D
Signal(s) : FID1A.ch
Acq On : 15 Mar 2019 14:19
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 15 23:54:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

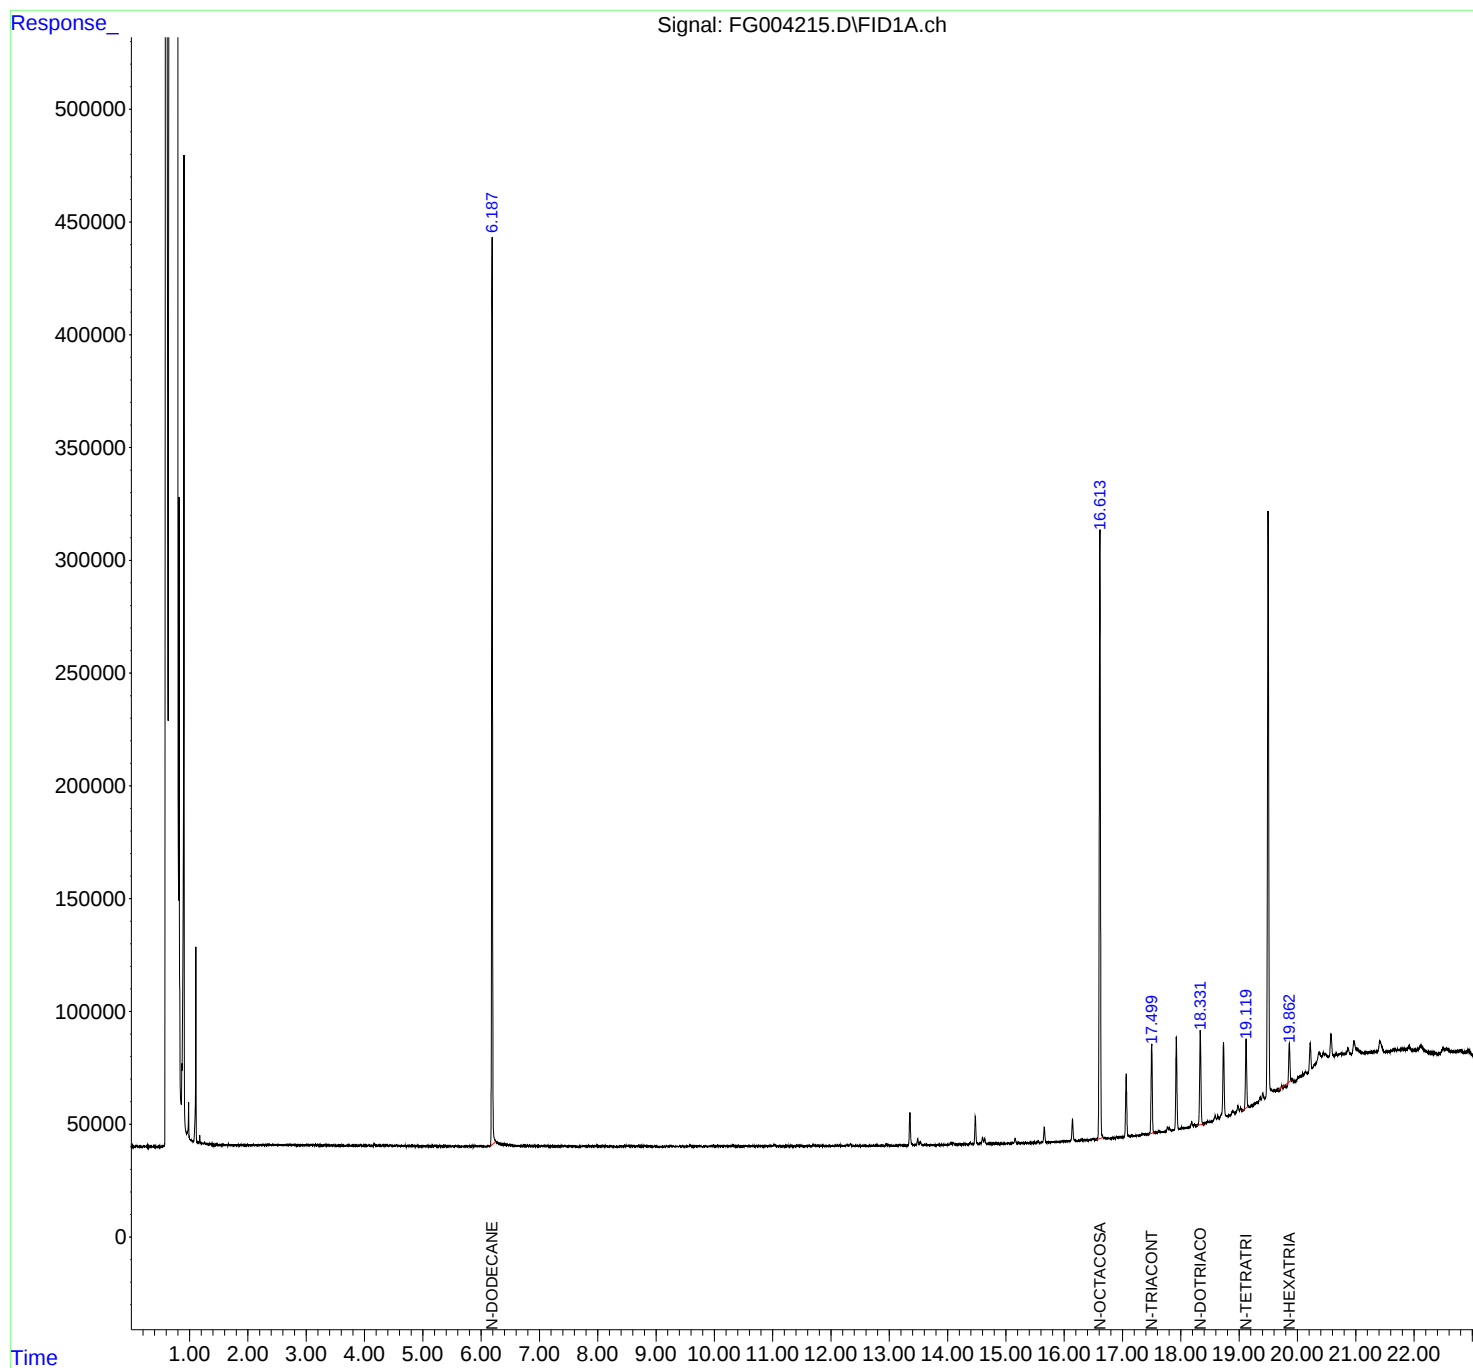


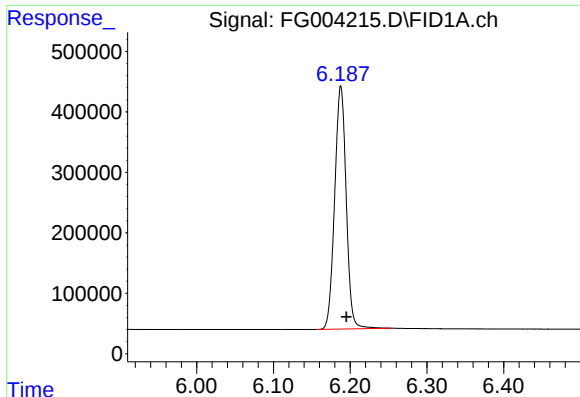

#3 N-DODECANE


R.T.: 6.188 min
Delta R.T.: -0.007 min
Response: 4192651
Conc: 30.93 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

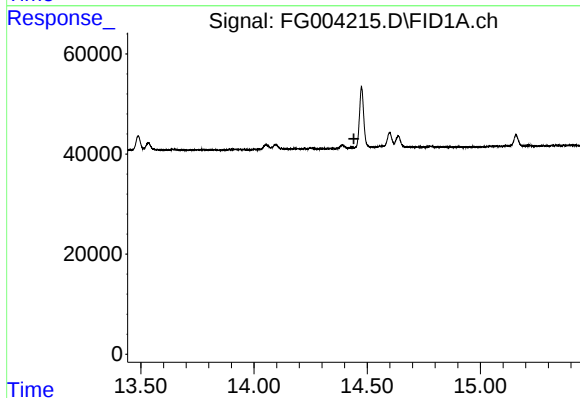


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.441 min
Response: 0
Conc: N.D.

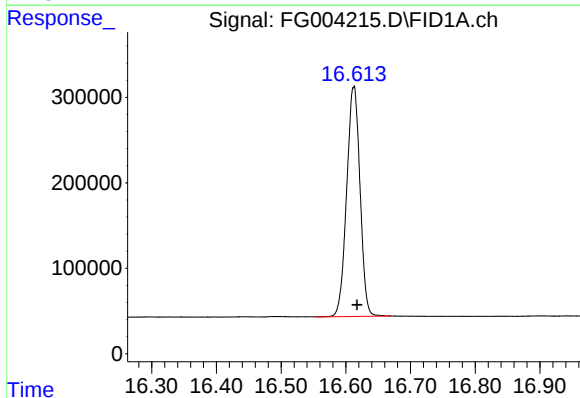


#12 N-OCTACOSANE

R.T.: 16.612 min
Delta R.T.: -0.005 min
Response: 3861165
Conc: 28.20 ug/ml

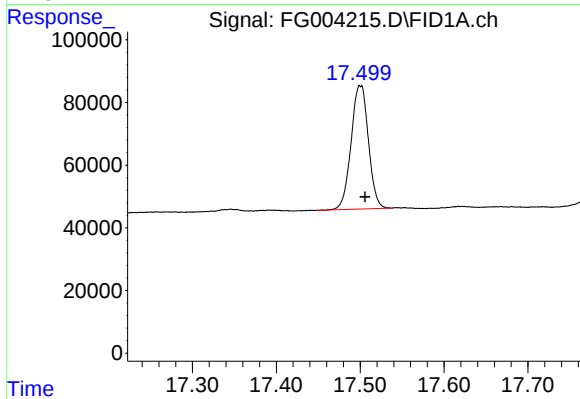

#13 N-TRIACONTANE


R.T.: 17.500 min
Delta R.T.: -0.005 min
Response: 563645
Conc: 4.22 ug/ml

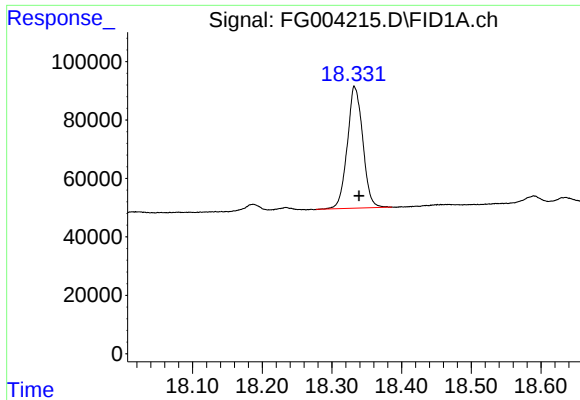

#14 N-DOTRIACONTANE


R.T.: 18.333 min
Delta R.T.: -0.007 min
Response: 642221
Conc: 5.08 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

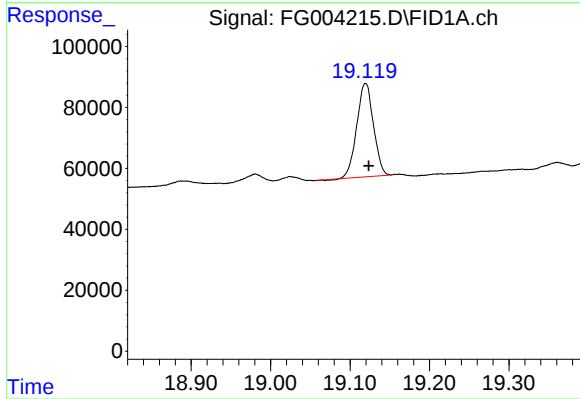

#15 N-TETRATRIACONTANE

R.T.: 19.120 min
Delta R.T.: -0.004 min
Response: 446190
Conc: 3.77 ug/ml

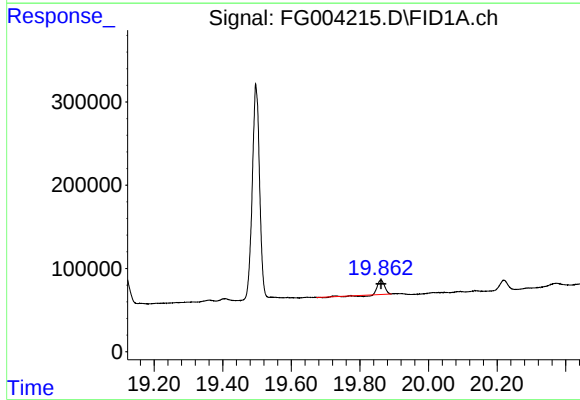

#16 N-HEXATRIACONTANE

R.T.: 19.862 min
Delta R.T.: 0.000 min
Response: 207720
Conc: 1.88 ug/ml