

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031619\
 Data File : FG004228.D
 Signal(s) : FID1A.ch
 Acq On : 15 Mar 2019 21:07
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Mar 15 23:57:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
 Quant Title :
 QLast Update : Tue Mar 05 03:05:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.443	1887834	15.016 ug/ml
Target Compounds			
15) N-TETRATRIACONTANE	19.131	165471	1.396 ug/ml
16) N-HEXATRIACONTANE	19.900	794328	7.175 ug/ml
17) N-OCTATRIACONTANE	20.586	725288	7.185 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031619\
Data File : FG004228.D
Signal(s) : FID1A.ch
Acq On : 15 Mar 2019 21:07
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 15 23:57:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

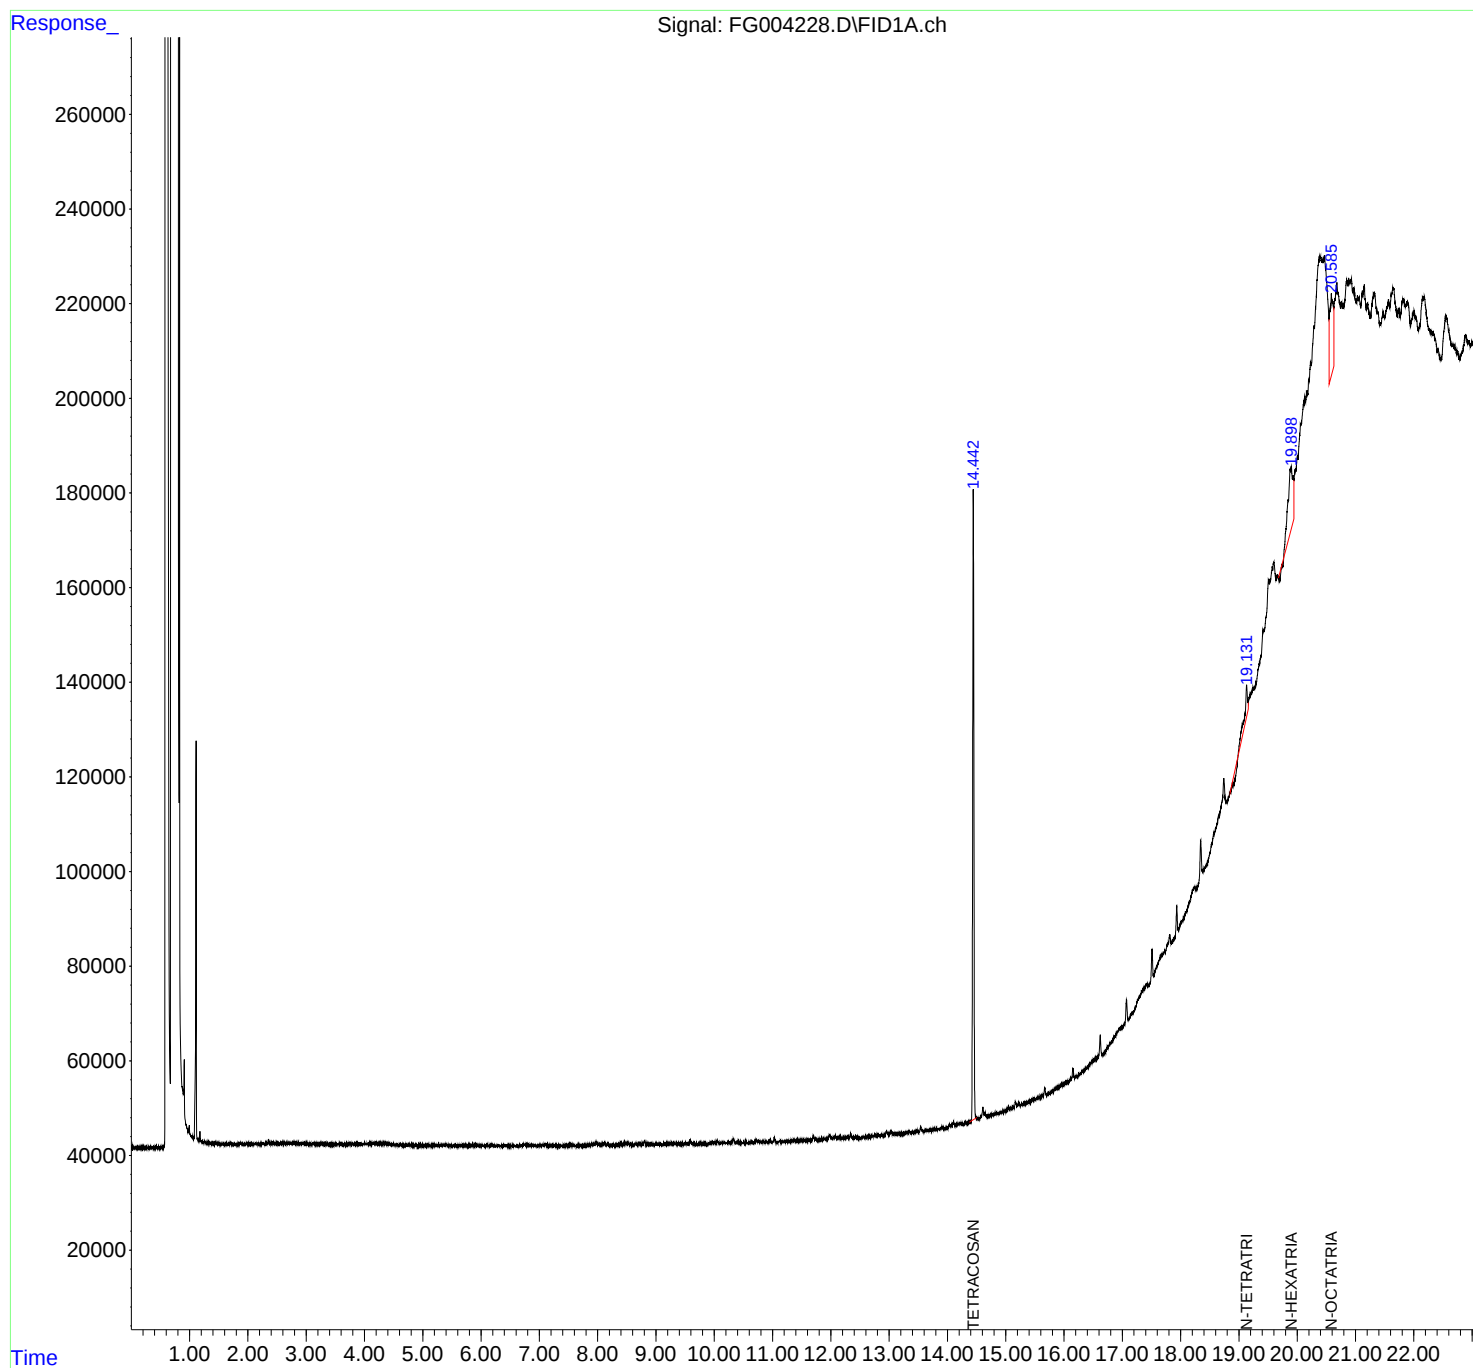


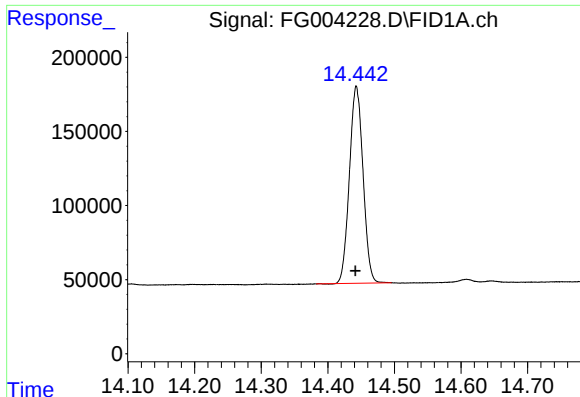

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.443 min
Delta R.T.: 0.002 min
Response: 1887834
Conc: 15.02 ug/ml

Instrument :
FID_G
ClientSampleId :
I.BLK

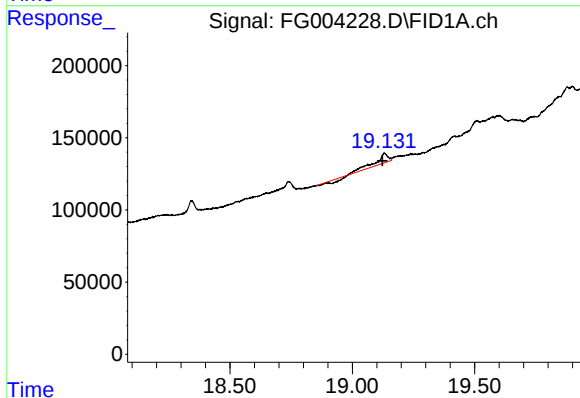


#15 N-TETRATRIACONTANE

R.T.: 19.131 min
Delta R.T.: 0.008 min
Response: 165471
Conc: 1.40 ug/ml

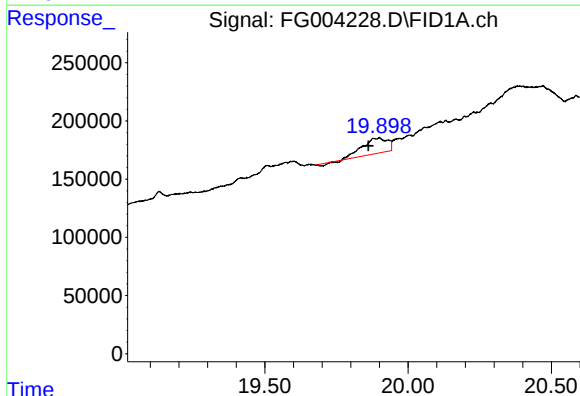

#16 N-HEXATRIACONTANE

R.T.: 19.900 min
Delta R.T.: 0.038 min
Response: 794328
Conc: 7.18 ug/ml

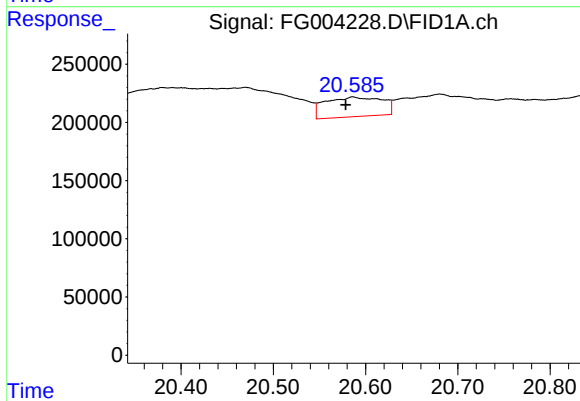

#17 N-OCTATRIACONTANE

R.T.: 20.586 min
Delta R.T.: 0.008 min
Response: 725288
Conc: 7.18 ug/ml