

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031619\
 Data File : FG004230.D
 Signal(s) : FID1A.ch
 Acq On : 15 Mar 2019 22:08
 Operator : AJ\SJ
 Sample : K1911-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 RBR200036

Integration File: autoint1.e
 Quant Time: Mar 15 23:58:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
 Quant Title :
 QLast Update : Tue Mar 05 03:05:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.441	1493394	11.879 ug/ml
Target Compounds			
4) N-TETRADECANE	8.045f	218626	1.568 ug/ml
7) N-EICOSANE	12.389	525986	3.682 ug/ml
10) N-TETRACOSANE	14.618	362701	2.572 ug/ml
12) N-OCTACOSANE	16.619	222169	1.623 ug/ml
13) N-TRIACONTANE	17.507	325880	2.440 ug/ml
14) N-DOTRIACONTANE	18.339	419946	3.319 ug/ml
15) N-TETRATRIACONTANE	19.131	156858	1.324 ug/ml
16) N-HEXATRIACONTANE	19.902	534911	4.832 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031619\
Data File : FG004230.D
Signal(s) : FID1A.ch
Acq On : 15 Mar 2019 22:08
Operator : AJ\SJ
Sample : K1911-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RBR200036

Integration File: autoint1.e
Quant Time: Mar 15 23:58:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

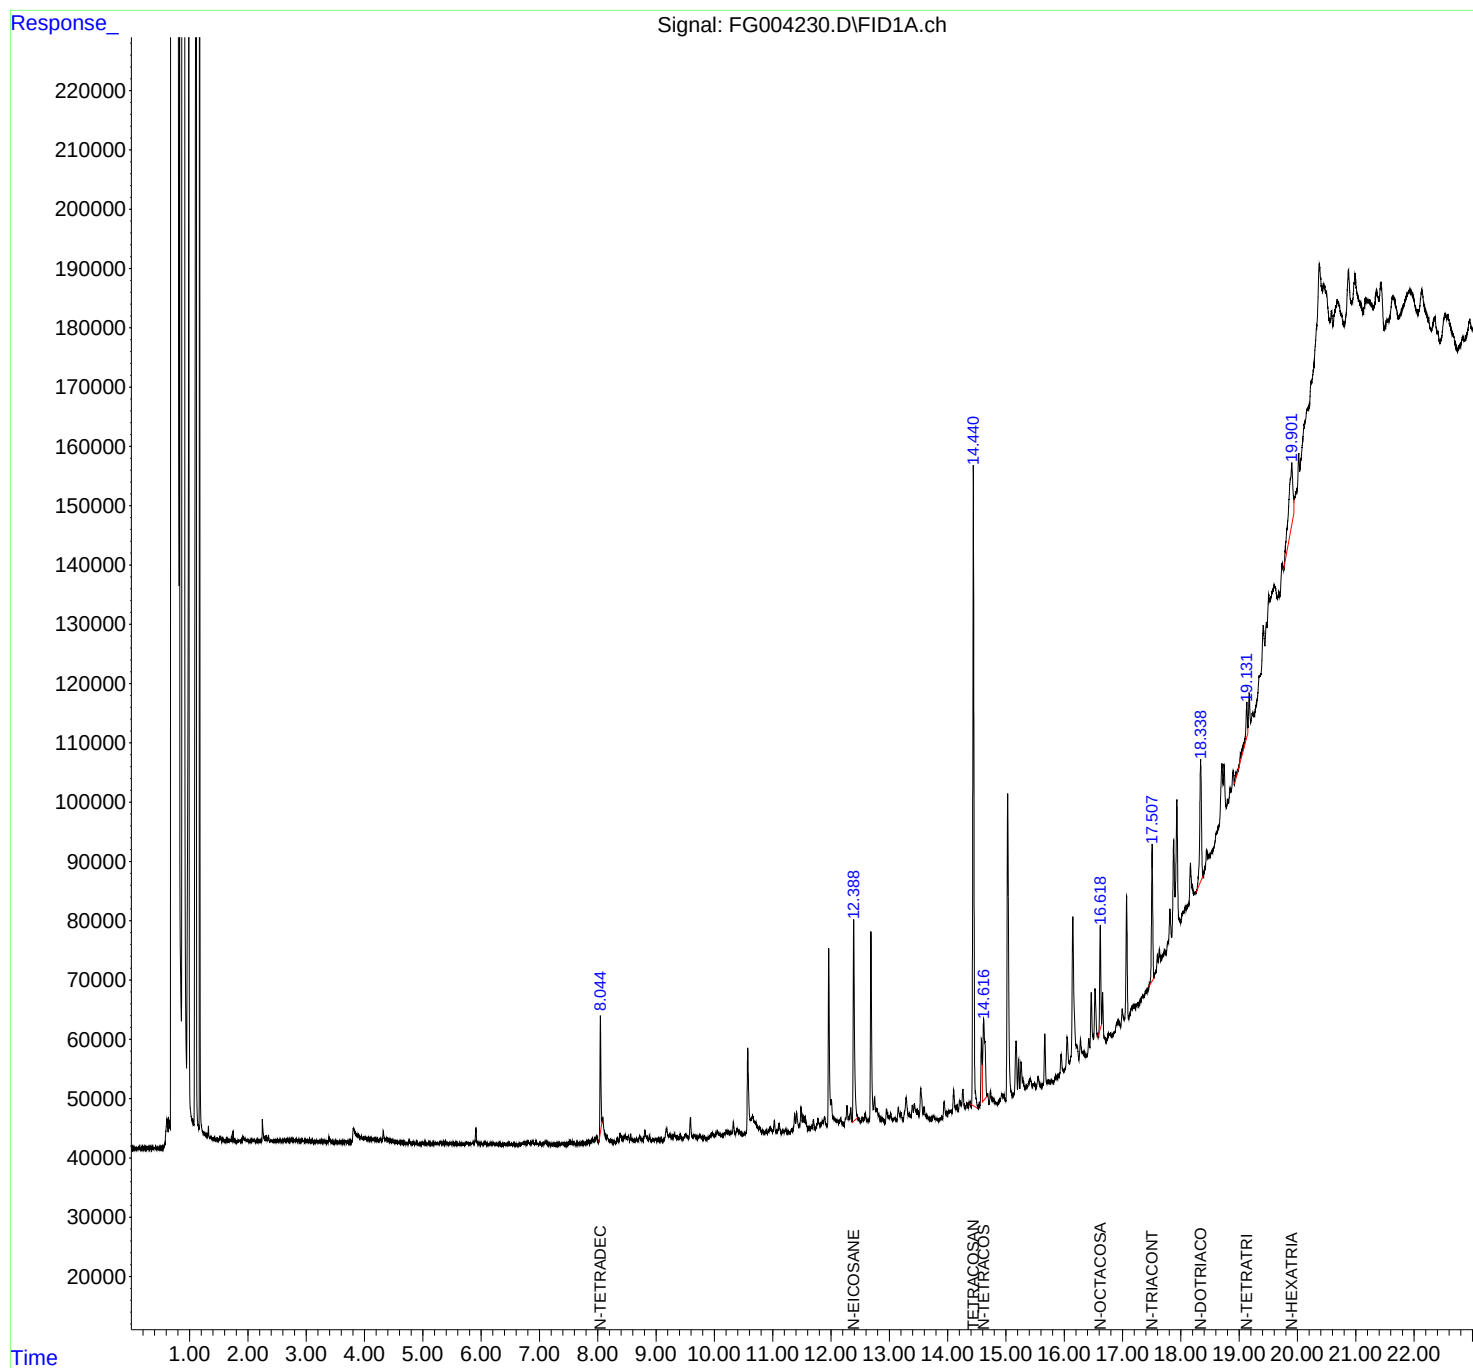


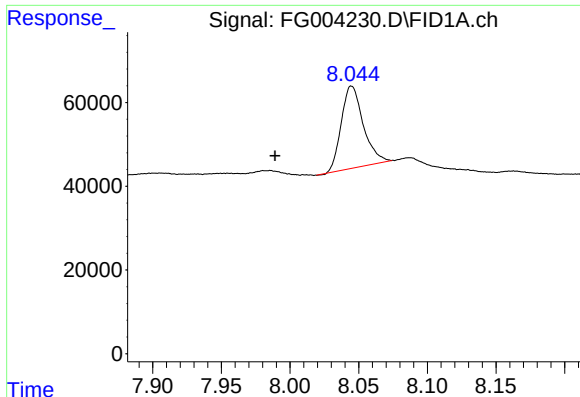

#4 N-TETRADECANE


R.T.: 8.045 min
Delta R.T.: 0.056 min
Response: 218626
Conc: 1.57 ug/ml

Instrument :
FID_G
ClientSampleId :
RBR200036

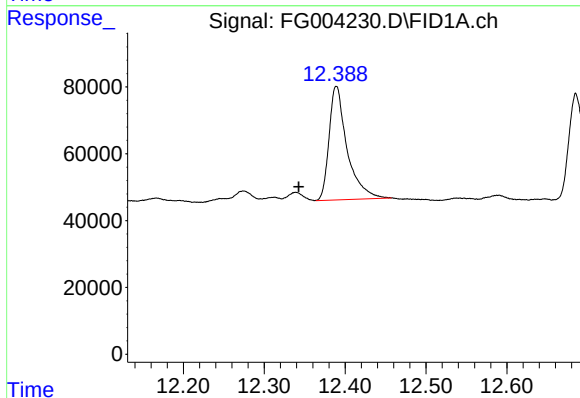


#7 N-EICOSANE

R.T.: 12.389 min
Delta R.T.: 0.047 min
Response: 525986
Conc: 3.68 ug/ml

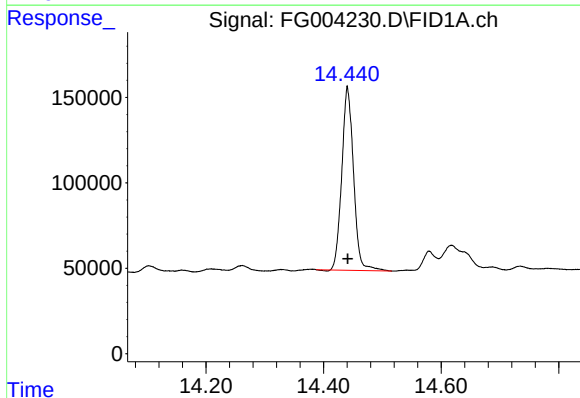


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.441 min
Delta R.T.: 0.000 min
Response: 1493394
Conc: 11.88 ug/ml

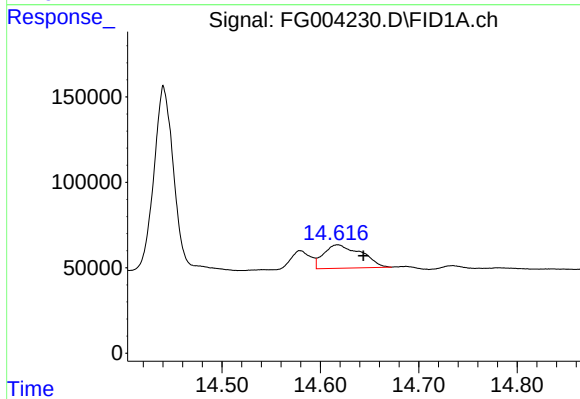

#10 N-TETRACOSANE


R.T.: 14.618 min
Delta R.T.: -0.026 min
Response: 362701
Conc: 2.57 ug/ml

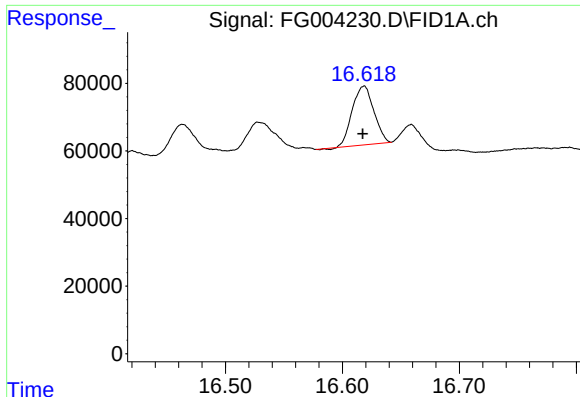

#12 N-OCTACOSANE


R.T.: 16.619 min
Delta R.T.: 0.000 min
Response: 222169
Conc: 1.62 ug/ml

Instrument :
FID_G
ClientSampleId :
RBR200036

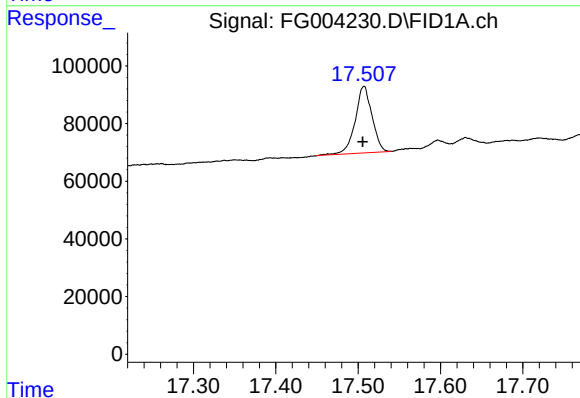


#13 N-TRIACONTANE

R.T.: 17.507 min
Delta R.T.: 0.001 min
Response: 325880
Conc: 2.44 ug/ml

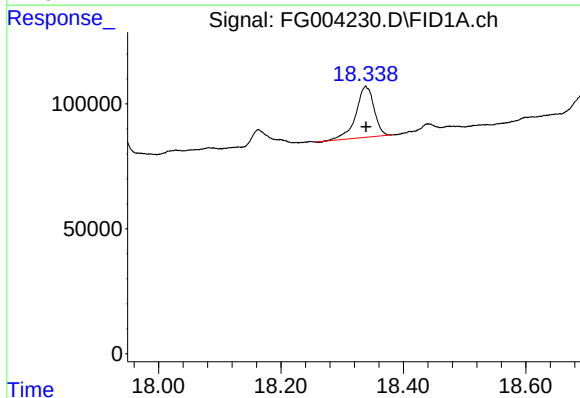


#14 N-DOTRIACONTANE

R.T.: 18.339 min
Delta R.T.: 0.000 min
Response: 419946
Conc: 3.32 ug/ml

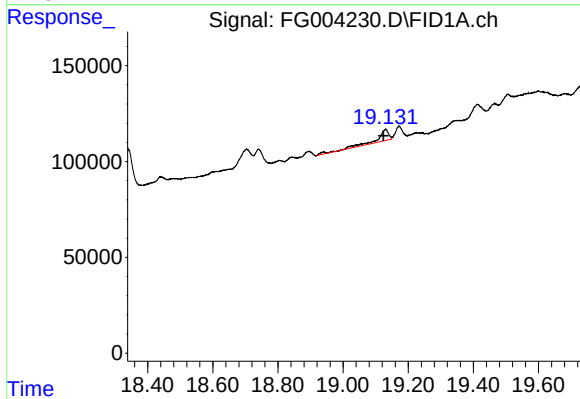

#15 N-TETRATRIACONTANE

R.T.: 19.131 min
Delta R.T.: 0.007 min
Response: 156858
Conc: 1.32 ug/ml

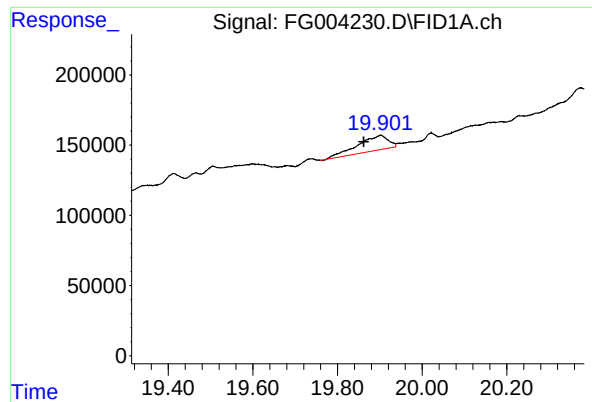

#16 N-HEXATRIACONTANE

R.T.: 19.902 min
Delta R.T.: 0.040 min
Response: 534911
Conc: 4.83 ug/ml

Instrument :
FID_G
ClientSampleId :
RBR200036