

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031619\
 Data File : FG004234.D
 Signal(s) : FID1A.ch
 Acq On : 16 Mar 2019 00:11
 Operator : AJ\SJ
 Sample : K1897-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 TP-1-B

Integration File: autoint1.e
 Quant Time: Mar 16 03:54:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
 Quant Title :
 QLast Update : Tue Mar 05 03:05:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.442	2098008	16.688 ug/ml
Target Compounds			
4) N-TETRADECANE	8.044f	371651	2.665 ug/ml
12) N-OCTACOSANE	16.618	391590	2.860 ug/ml
13) N-TRIACONTANE	17.507	589586	4.415 ug/ml
14) N-DOTRIACONTANE	18.339	630258	4.981 ug/ml
15) N-TETRATRIACONTANE	19.169	242354	2.045 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031619\
Data File : FG004234.D
Signal(s) : FID1A.ch
Acq On : 16 Mar 2019 00:11
Operator : AJ\SJ
Sample : K1897-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
TP-1-B

Integration File: autoint1.e
Quant Time: Mar 16 03:54:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

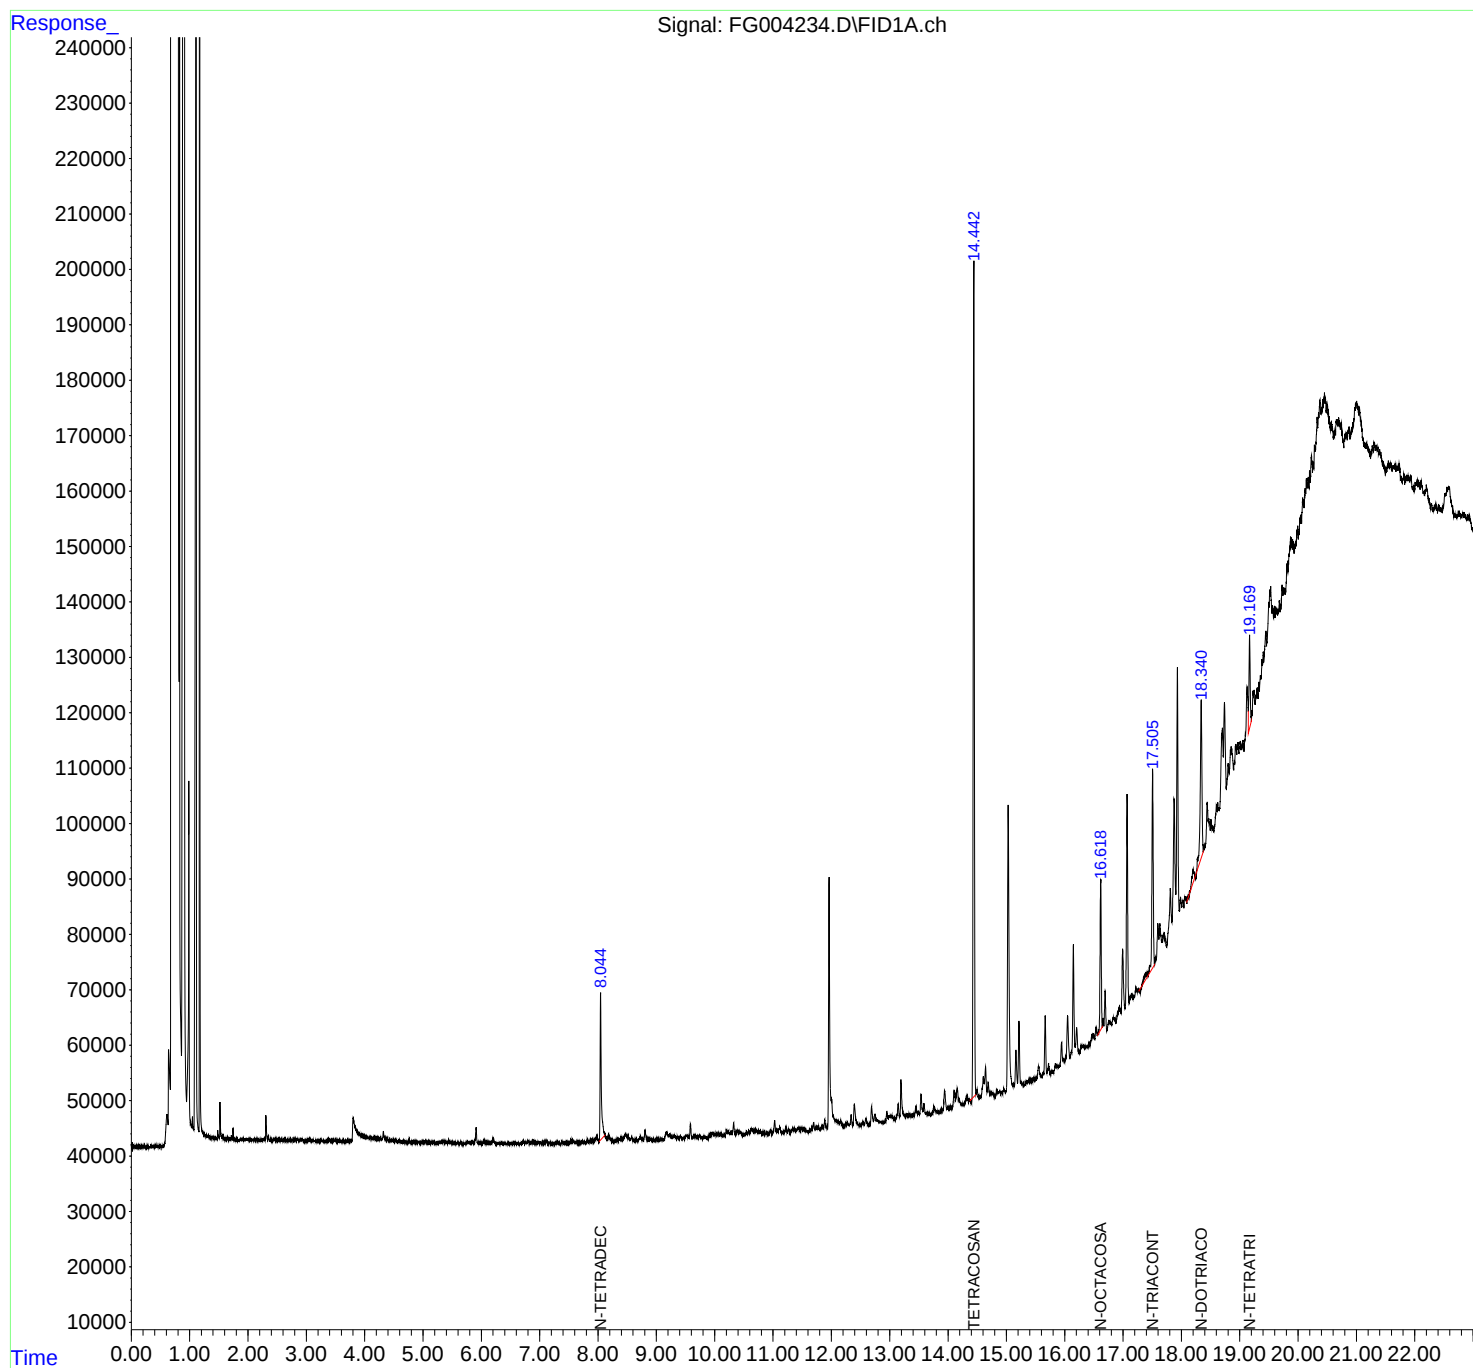


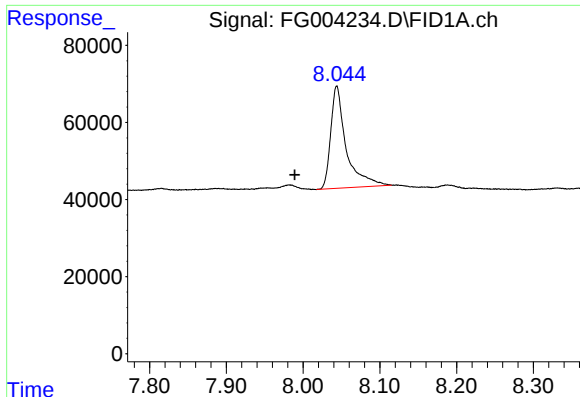

#4 N-TETRADECANE


R.T.: 8.044 min
Delta R.T.: 0.055 min
Response: 371651
Conc: 2.67 ug/ml

Instrument :
FID_G
ClientSampleId :
TP-1-B

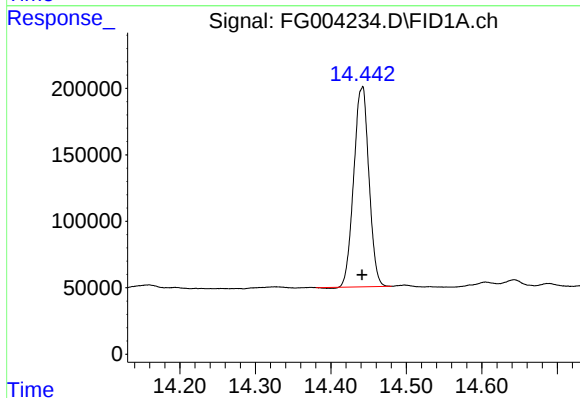


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.442 min
Delta R.T.: 0.000 min
Response: 2098008
Conc: 16.69 ug/ml

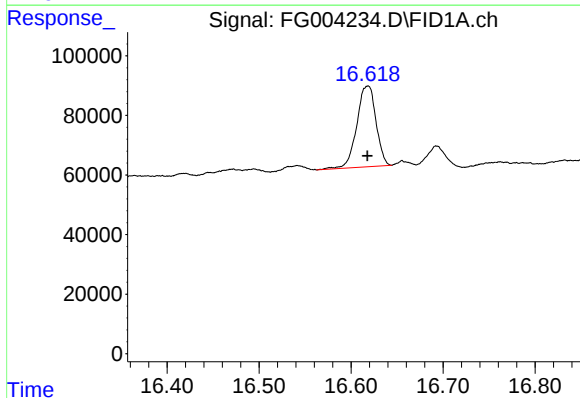


#12 N-OCTACOSANE

R.T.: 16.618 min
Delta R.T.: 0.000 min
Response: 391590
Conc: 2.86 ug/ml

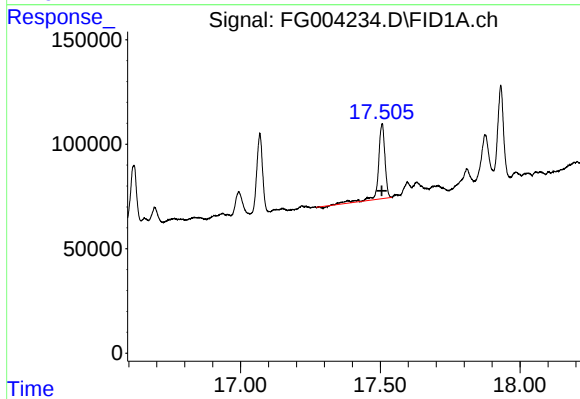

#13 N-TRIACONTANE


R.T.: 17.507 min
Delta R.T.: 0.000 min
Response: 589586
Conc: 4.41 ug/ml

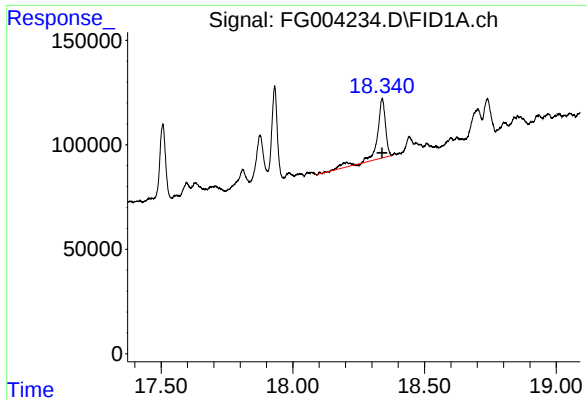

#14 N-DOTRIACONTANE

R.T.: 18.339 min
Delta R.T.: 0.000 min
Response: 630258
Conc: 4.98 ug/ml

Instrument :
FID_G
ClientSampleId :
TP-1-B

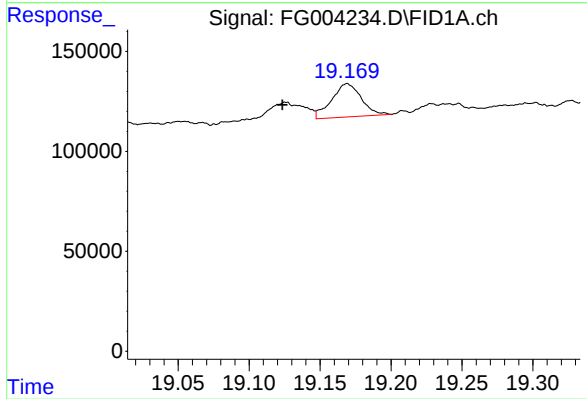

#15 N-TETRATRIACONTANE

R.T.: 19.169 min
Delta R.T.: 0.045 min
Response: 242354
Conc: 2.05 ug/ml