

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031619\
Data File : FG004236.D
Signal(s) : FID1A.ch
Acq On : 16 Mar 2019 01:12
Operator : AJ\SJ
Sample : K1897-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
TP-2-B

Integration File: autoint1.e
Quant Time: Mar 16 03:55:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.437	1143466	9.095 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.616	299582	2.188 ug/ml
13) N-TRIACONTANE	17.505	405328	3.035 ug/ml
14) N-DOTRIACONTANE	18.334	539714	4.265 ug/ml
16) N-HEXATRIACONTANE	19.900	365939	3.305 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031619\
Data File : FG004236.D
Signal(s) : FID1A.ch
Acq On : 16 Mar 2019 01:12
Operator : AJ\SJ
Sample : K1897-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
TP-2-B

Integration File: autoint1.e
Quant Time: Mar 16 03:55:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

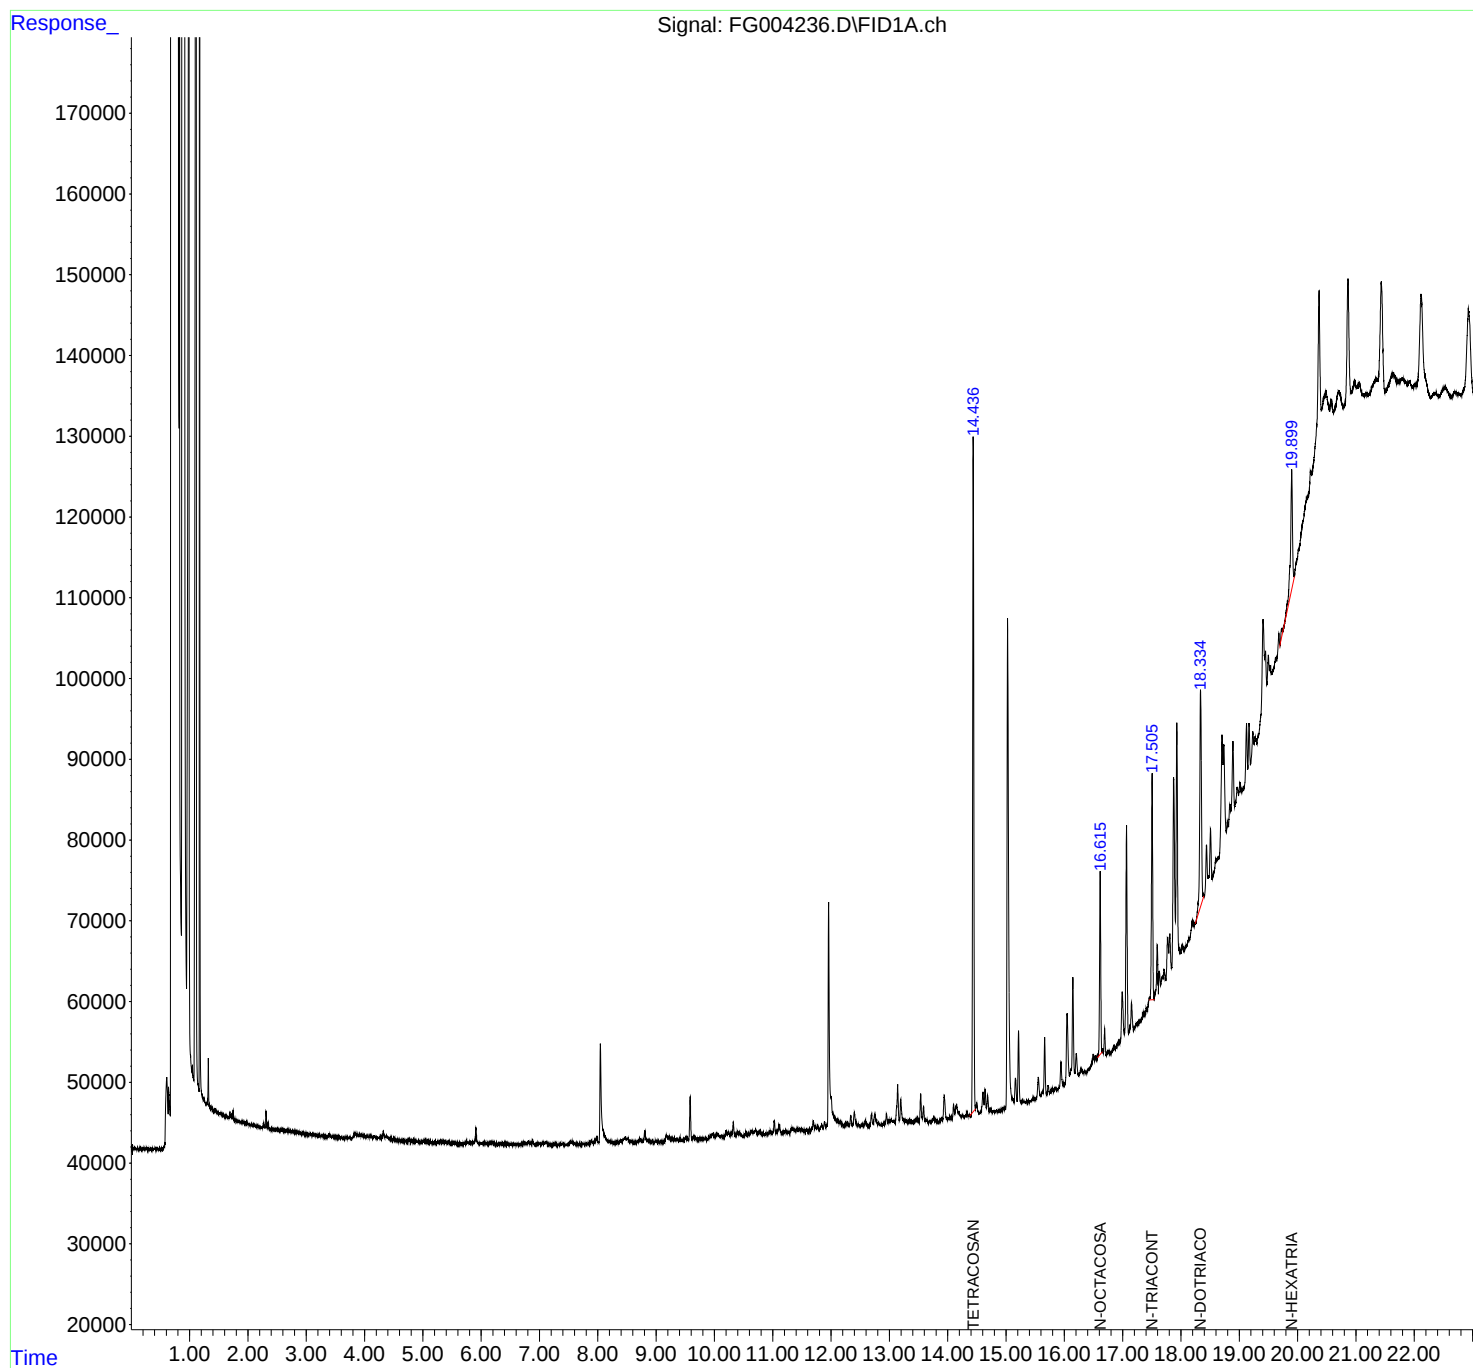


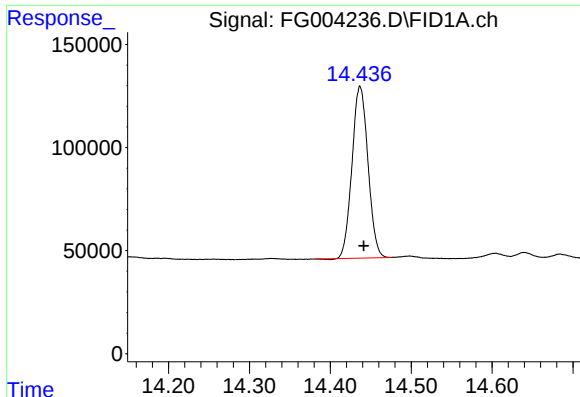

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.437 min
Delta R.T.: -0.004 min
Response: 1143466
Conc: 9.10 ug/ml

Instrument :
FID_G
ClientSampleId :
TP-2-B

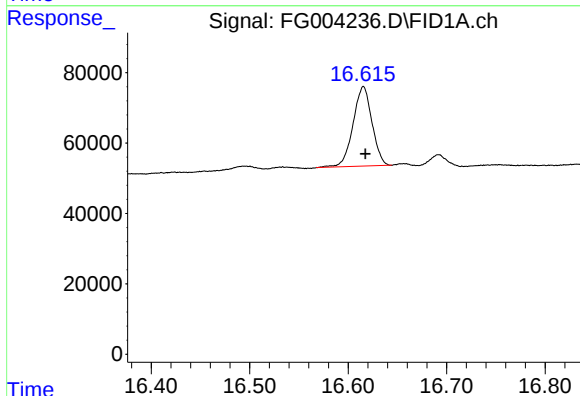


#12 N-OCTACOSANE

R.T.: 16.616 min
Delta R.T.: -0.002 min
Response: 299582
Conc: 2.19 ug/ml

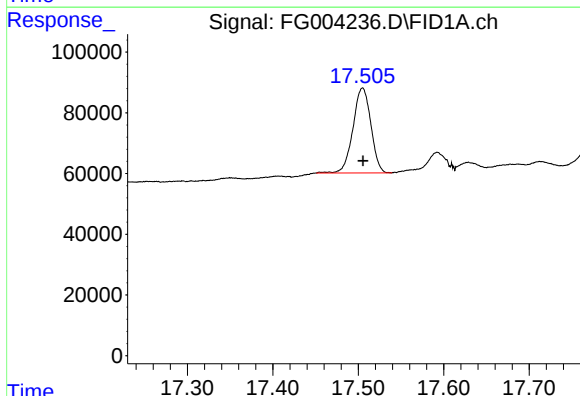


#13 N-TRIACONTANE

R.T.: 17.505 min
Delta R.T.: 0.000 min
Response: 405328
Conc: 3.04 ug/ml

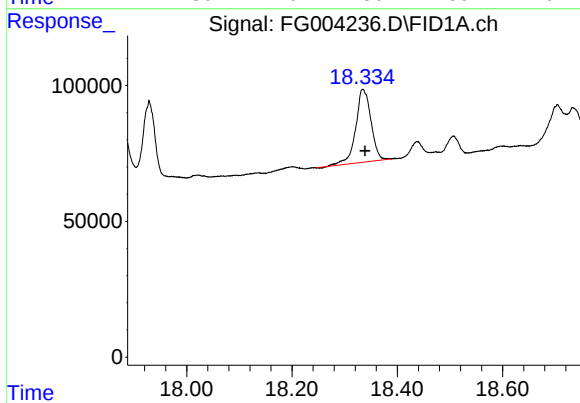

#14 N-DOTRIACONTANE

R.T.: 18.334 min
Delta R.T.: -0.005 min
Response: 539714
Conc: 4.27 ug/ml

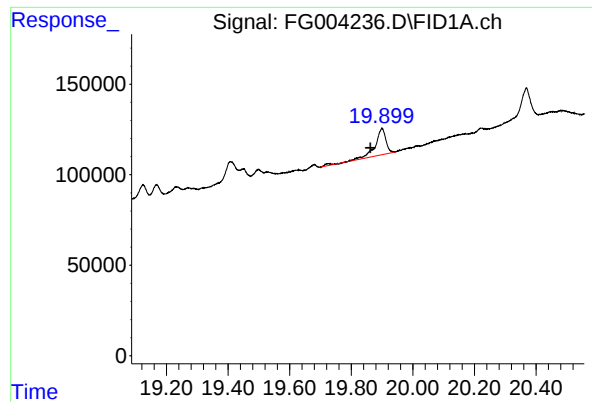

#16 N-HEXATRIACONTANE

R.T.: 19.900 min
Delta R.T.: 0.038 min
Response: 365939
Conc: 3.31 ug/ml

Instrument :
FID_G
ClientSampleId :
TP-2-B