

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031619\
Data File : FG004241.D
Signal(s) : FID1A.ch
Acq On : 16 Mar 2019 03:44
Operator : AJ\SJ
Sample : K1685-01 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
AU-05-031419-A

Integration File: autoint1.e
Quant Time: Mar 16 05:42:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.338	286708	2.266 ug/ml
16)	N-HEXATRIACONTANE	19.901	416287	3.760 ug/ml
18)	N-TETRACONTANE	21.438	570601	5.380 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031619\
Data File : FG004241.D
Signal(s) : FID1A.ch
Acq On : 16 Mar 2019 03:44
Operator : AJ\SJ
Sample : K1685-01 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
AU-05-031419-A

Integration File: autoint1.e
Quant Time: Mar 16 05:42:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

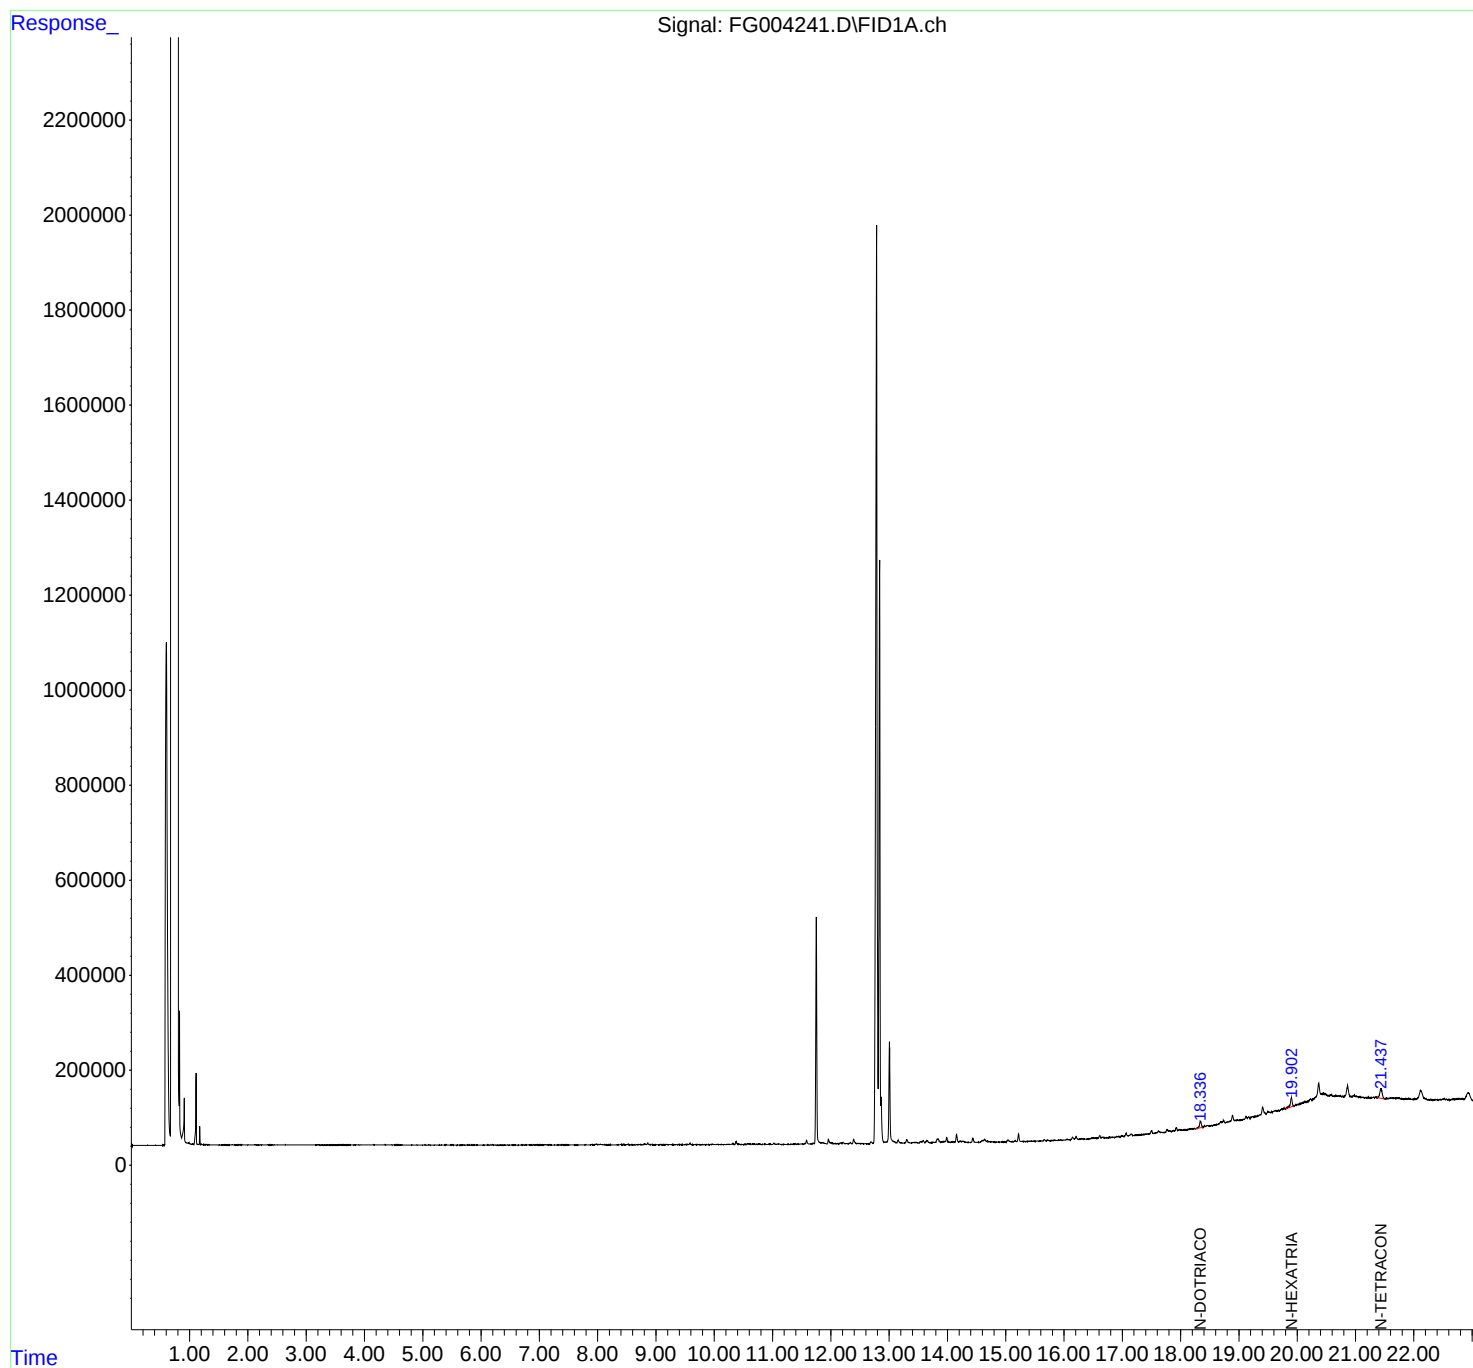


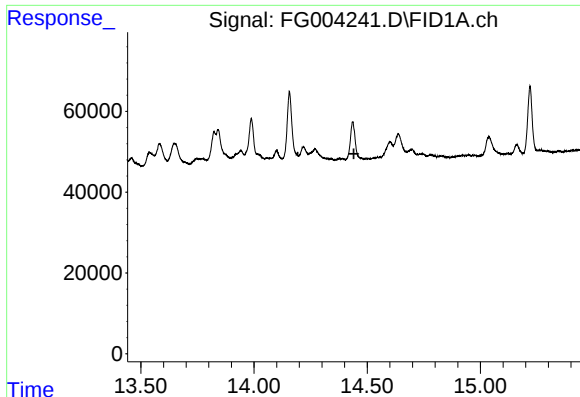

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.441 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :
AU-05-031419-A

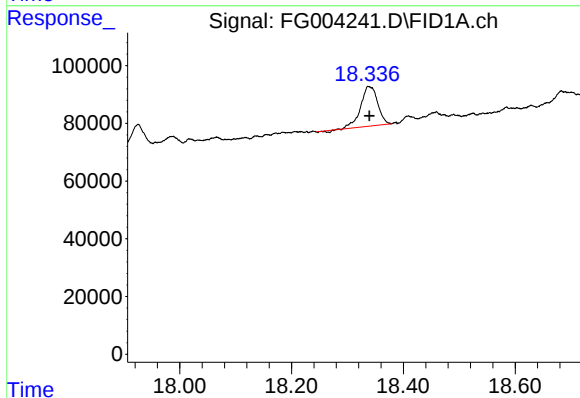


#14 N-DOTRIACONTANE

R.T.: 18.338 min
Delta R.T.: -0.001 min
Response: 286708
Conc: 2.27 ug/ml

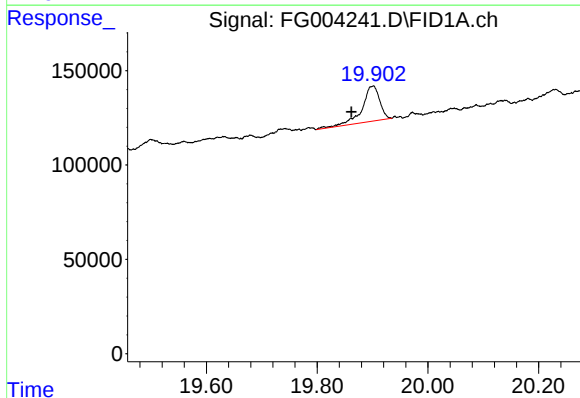

#16 N-HEXATRIACONTANE

R.T.: 19.901 min
Delta R.T.: 0.040 min
Response: 416287
Conc: 3.76 ug/ml

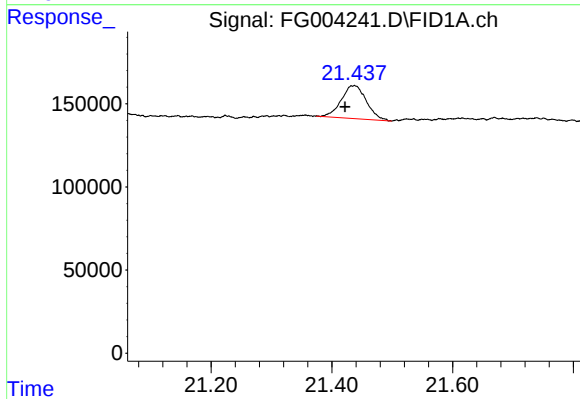

#18 N-TETRACONTANE

R.T.: 21.438 min
Delta R.T.: 0.016 min
Response: 570601
Conc: 5.38 ug/ml