

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031619\
Data File : FG004244.D
Signal(s) : FID1A.ch
Acq On : 16 Mar 2019 05:15
Operator : AJ\SJ
Sample : K1698-01 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
TR-04-031419

Integration File: autoint1.e
Quant Time: Mar 16 05:42:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
4) N-TETRADECANE	7.926f	175364	1.258 ug/ml
7) N-EICOSANE	12.392	684412	4.791 ug/ml
8) N-DOCOSANE	13.583	1069252	7.533 ug/ml
10) N-TETRACOSANE	14.632	1052723	7.465 ug/ml
14) N-DOTRIACONTANE	18.343	423162	3.344 ug/ml
15) N-TETRATRIACONTANE	19.126	132458	1.118 ug/ml
16) N-HEXATRIACONTANE	19.901	570323	5.152 ug/ml
18) N-TETRACONTANE	21.438	546986	5.157 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031619\
Data File : FG004244.D
Signal(s) : FID1A.ch
Acq On : 16 Mar 2019 05:15
Operator : AJ\SJ
Sample : K1698-01 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
TR-04-031419

Integration File: autoint1.e
Quant Time: Mar 16 05:42:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

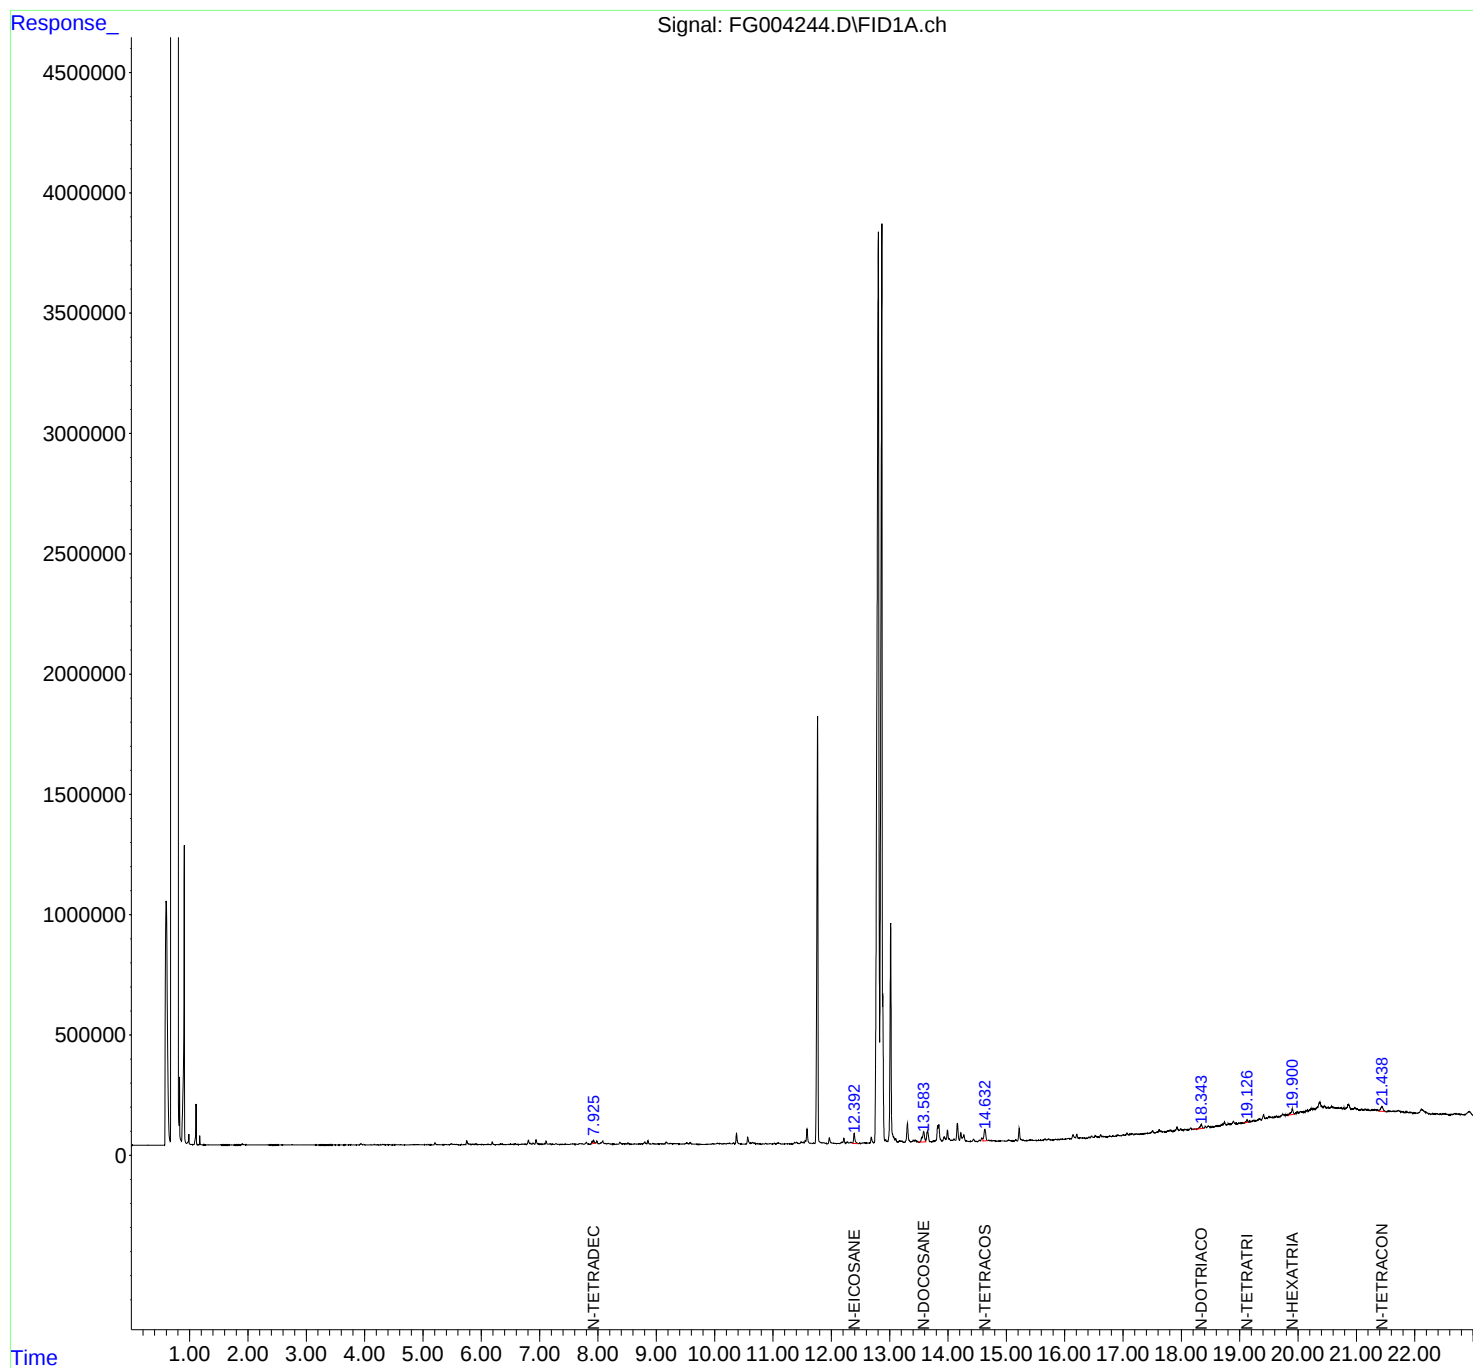


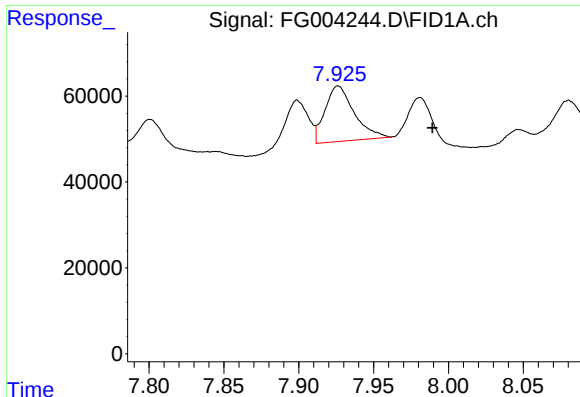

#4 N-TETRADECANE


R.T.: 7.926 min
Delta R.T.: -0.063 min
Response: 175364
Conc: 1.26 ug/ml

Instrument :
FID_G
ClientSampleId :
TR-04-031419

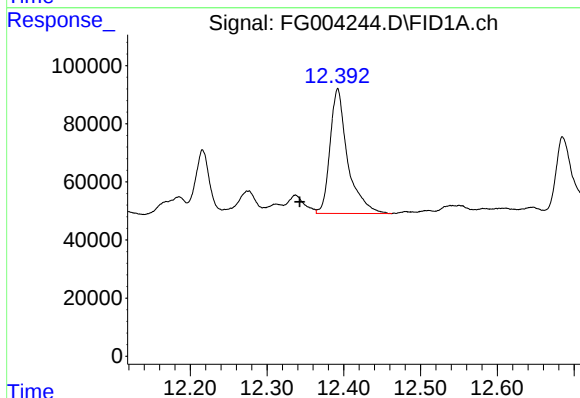


#7 N-EICOSANE

R.T.: 12.392 min
Delta R.T.: 0.050 min
Response: 684412
Conc: 4.79 ug/ml

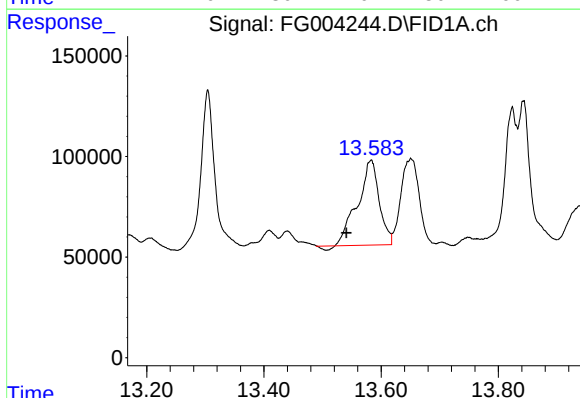


#8 N-DOCOSANE

R.T.: 13.583 min
Delta R.T.: 0.042 min
Response: 1069252
Conc: 7.53 ug/ml

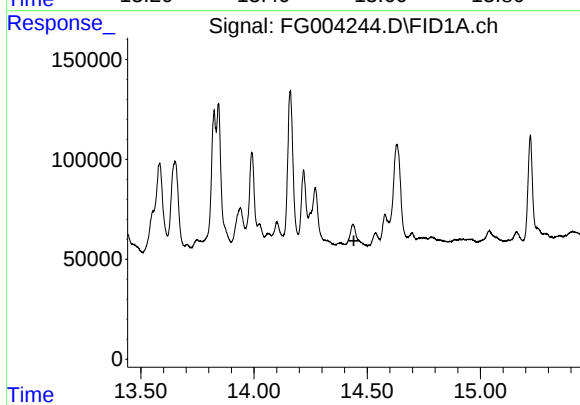

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.441 min
Response: 0
Conc: N.D.

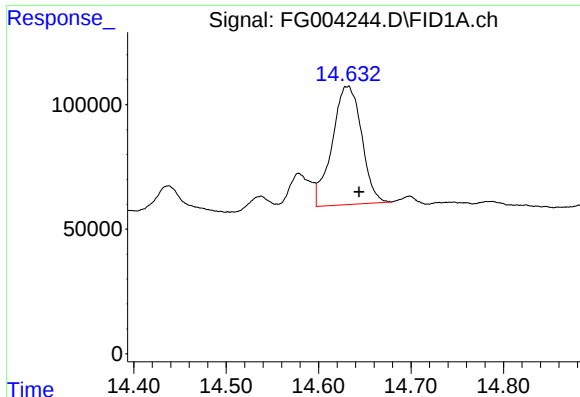

#10 N-TETRACOSANE


R.T.: 14.632 min
Delta R.T.: -0.012 min
Response: 1052723
Conc: 7.46 ug/ml

Instrument :
FID_G
ClientSampleId :
TR-04-031419

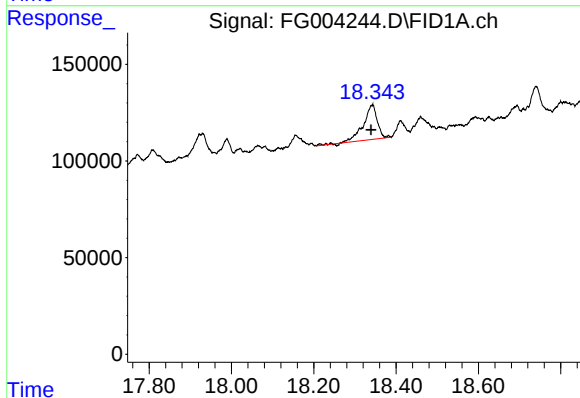


#14 N-DOTRIACONTANE

R.T.: 18.343 min
Delta R.T.: 0.004 min
Response: 423162
Conc: 3.34 ug/ml

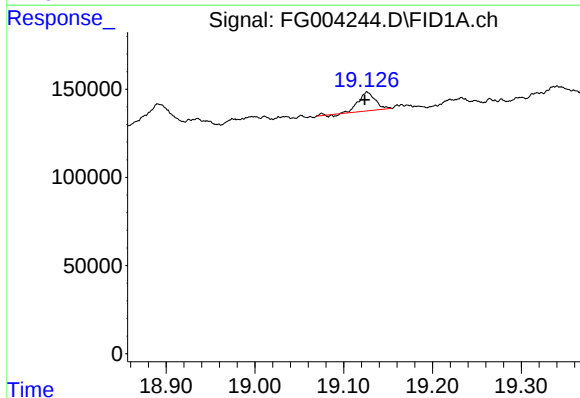


#15 N-TETRATRIACONTANE

R.T.: 19.126 min
Delta R.T.: 0.003 min
Response: 132458
Conc: 1.12 ug/ml

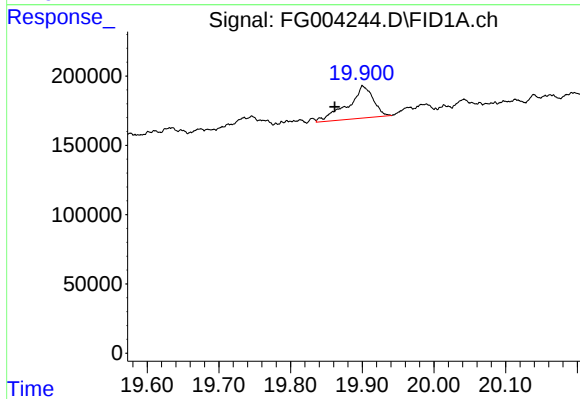

#16 N-HEXATRIACONTANE

R.T.: 19.901 min
Delta R.T.: 0.039 min
Response: 570323
Conc: 5.15 ug/ml

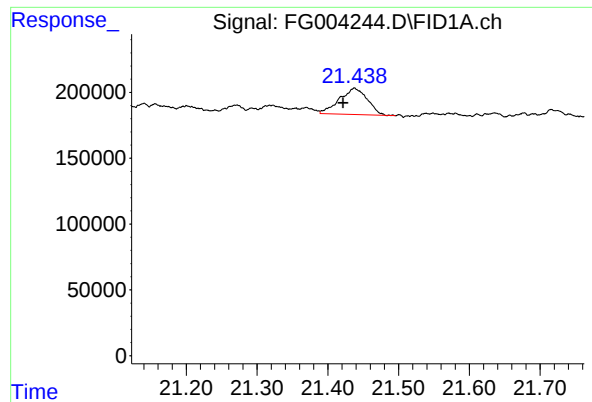

#18 N-TETRACONTANE

R.T.: 21.438 min
Delta R.T.: 0.016 min
Response: 546986
Conc: 5.16 ug/ml

Instrument :
FID_G
ClientSampleId :
TR-04-031419