

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031619\
 Data File : FG004245.D
 Signal(s) : FID1A.ch
 Acq On : 16 Mar 2019 05:45
 Operator : AJ\SJ
 Sample : K1901-05 10X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 SB-4(0.5-1.5)

Integration File: autoint1.e
 Quant Time: Mar 16 06:51:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
 Quant Title :
 QLast Update : Tue Mar 05 03:05:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.439	480157	3.819 ug/ml
Target Compounds			
7) N-EICOSANE	12.385	4282113	29.975 ug/ml
8) N-DOCOSANE	13.549	701387	4.941 ug/ml
10) N-TETRACOSANE	14.610	2734862	19.392 ug/ml
12) N-OCTACOSANE	16.621	666987	4.872 ug/ml
13) N-TRIACONTANE	17.509	317199	2.375 ug/ml
14) N-DOTRIACONTANE	18.296	200229	1.582 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031619\
Data File : FG004245.D
Signal(s) : FID1A.ch
Acq On : 16 Mar 2019 05:45
Operator : AJ\SJ
Sample : K1901-05 10X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SB-4(0.5-1.5)

Integration File: autoint1.e
Quant Time: Mar 16 06:51:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

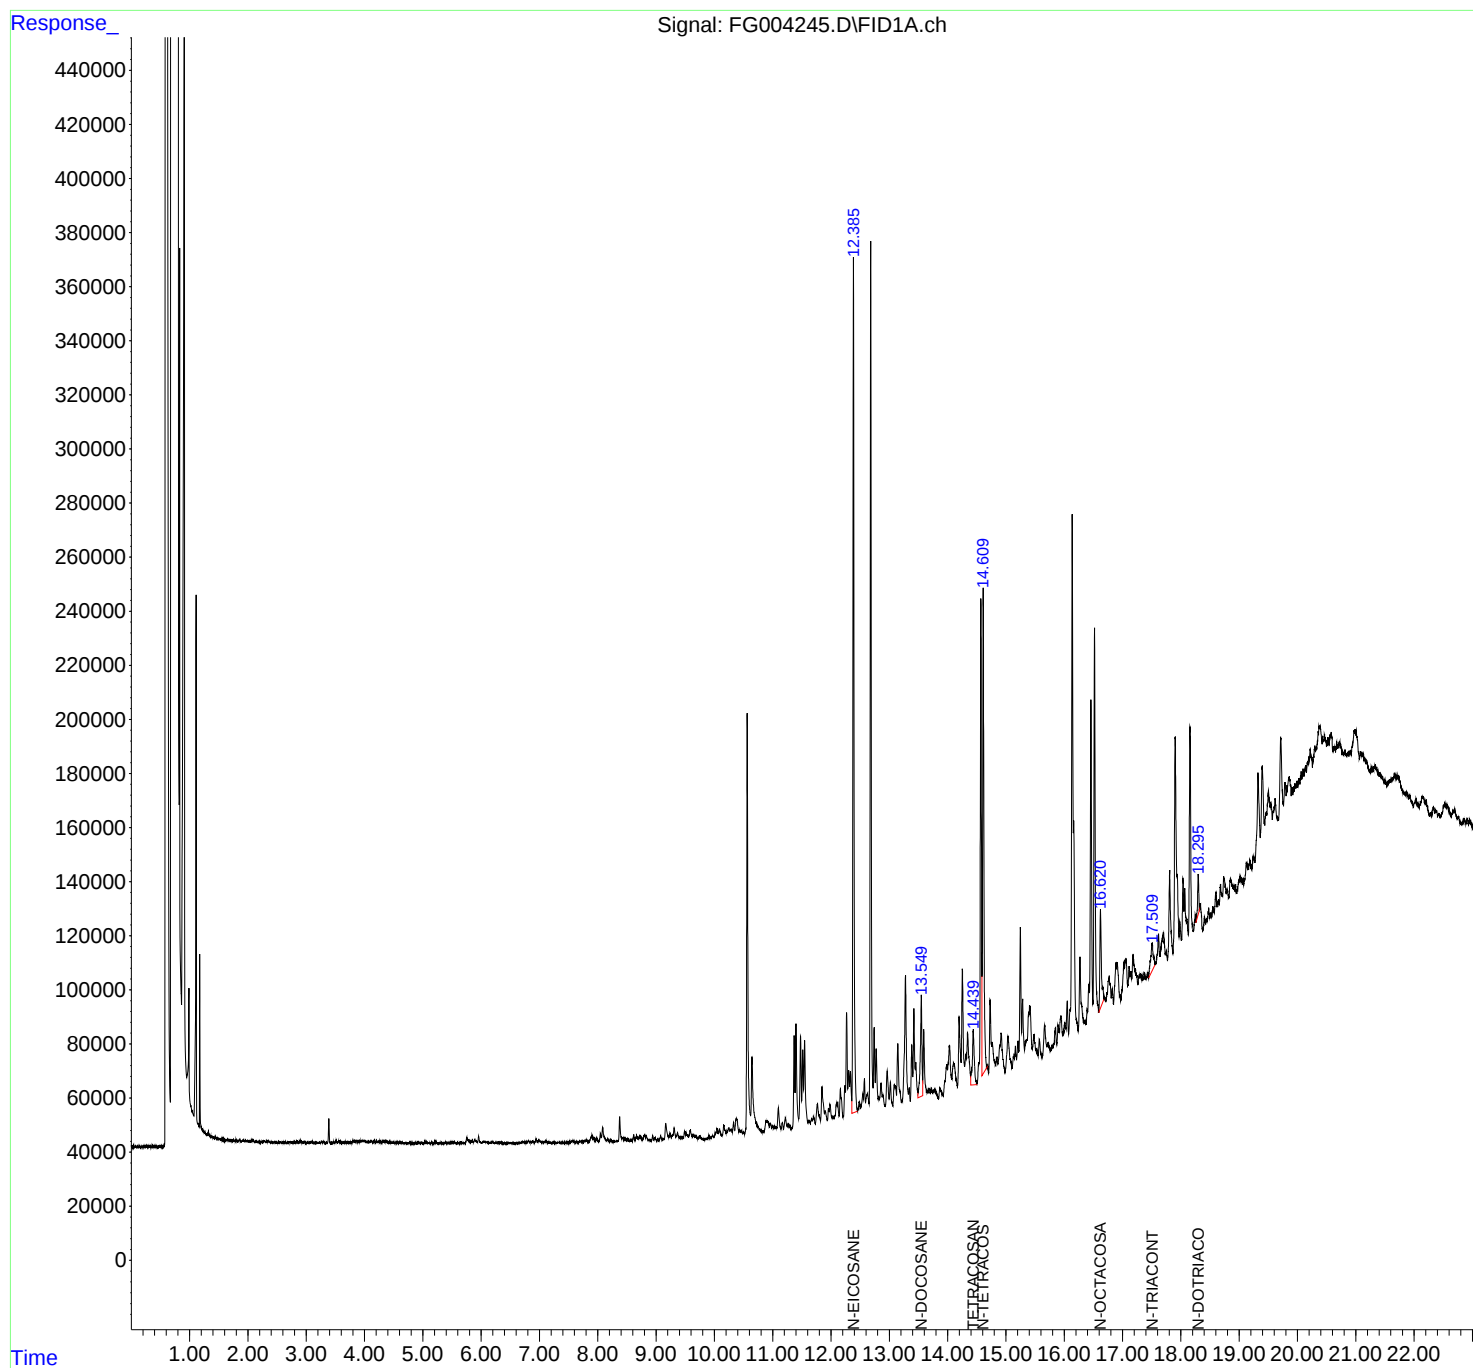


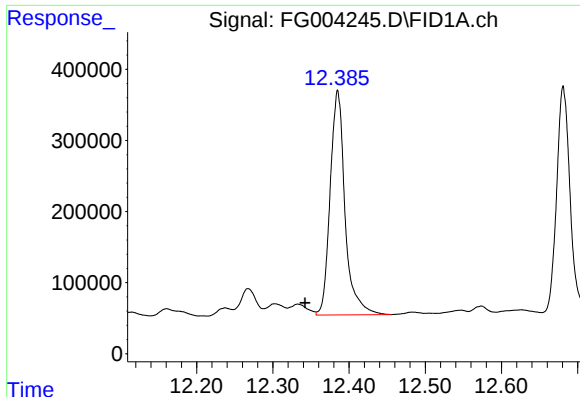

#7 N-EICOSANE


R.T.: 12.385 min
Delta R.T.: 0.043 min
Response: 4282113
Conc: 29.98 ug/ml

Instrument :
FID_G
ClientSampleId :
SB-4(0.5-1.5)

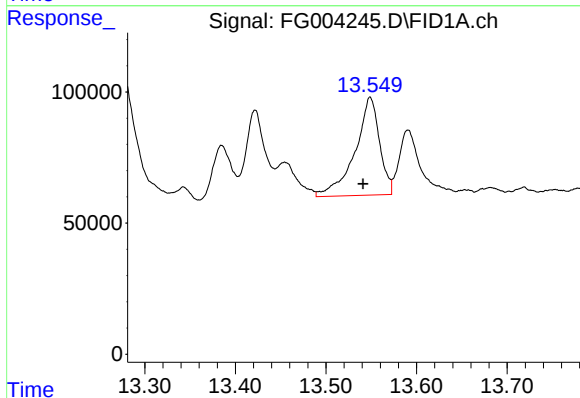


#8 N-DOCOSANE

R.T.: 13.549 min
Delta R.T.: 0.008 min
Response: 701387
Conc: 4.94 ug/ml

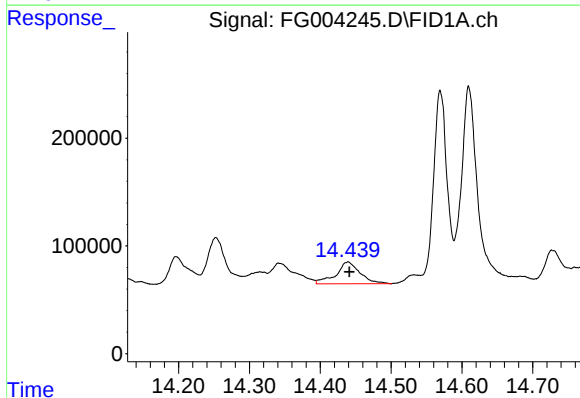


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.439 min
Delta R.T.: -0.002 min
Response: 480157
Conc: 3.82 ug/ml

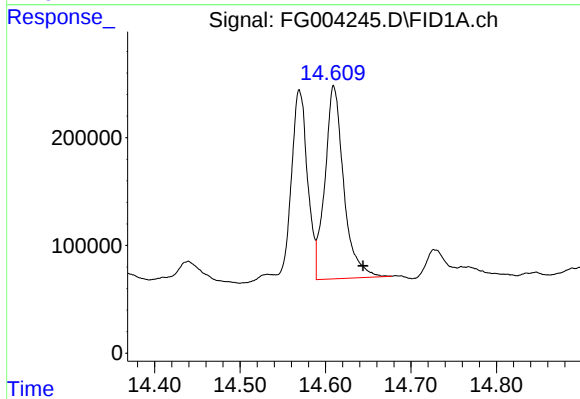

#10 N-TETRACOSANE


R.T.: 14.610 min
Delta R.T.: -0.034 min
Response: 2734862
Conc: 19.39 ug/ml

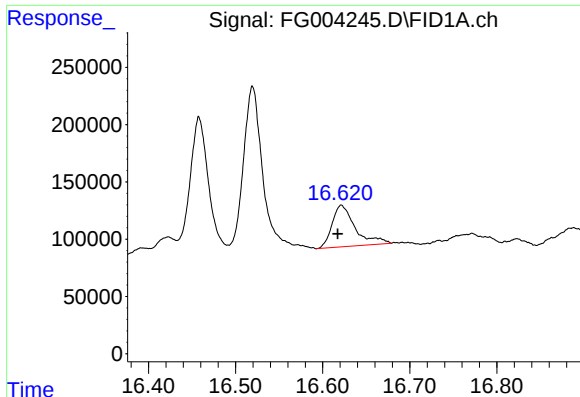

#12 N-OCTACOSANE


R.T.: 16.621 min
Delta R.T.: 0.004 min
Response: 666987
Conc: 4.87 ug/ml

Instrument :
FID_G
ClientSampleId :
SB-4(0.5-1.5)

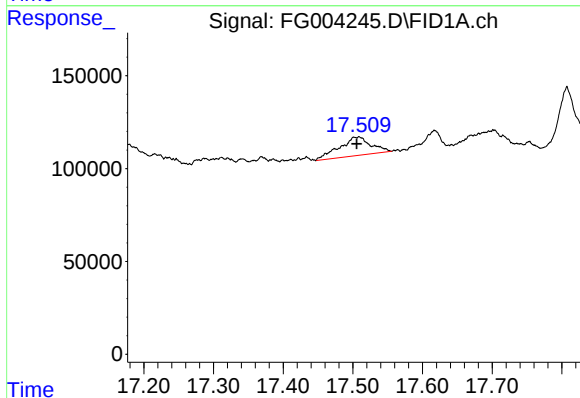

#13 N-TRIACONTANE

R.T.: 17.509 min
Delta R.T.: 0.003 min
Response: 317199
Conc: 2.38 ug/ml

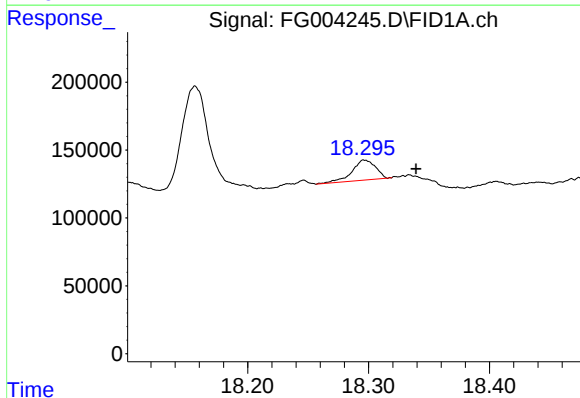

#14 N-DOTRIACONTANE

R.T.: 18.296 min
Delta R.T.: -0.043 min
Response: 200229
Conc: 1.58 ug/ml