

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031621\
 Data File : FG007709.D
 Signal(s) : FID1A.ch
 Acq On : 16 Mar 2021 10:51
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 17 01:12:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031221.M
 Quant Title :
 QLast Update : Mon Mar 15 09:29:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.191	4269912	28.827 ug/ml
6) N-OCTADECANE	11.032	83332	0.553 ug/ml
12) N-OCTACOSANE	16.630	4047792	29.599 ug/ml
13) N-TRIACONTANE	17.517	213801	1.616 ug/ml
14) N-DOTRIACONTANE	18.353	313596	2.489 ug/ml
15) N-TETRATRIACONTANE	19.139	200268	1.745 ug/ml
16) N-HEXATRIACONTANE	19.881	154915	1.531 ug/ml
18) N-TETRACONTANE	21.502f	306785	3.503 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031621\
Data File : FG007709.D
Signal(s) : FID1A.ch
Acq On : 16 Mar 2021 10:51
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 17 01:12:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031221.M
Quant Title :
QLast Update : Mon Mar 15 09:29:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

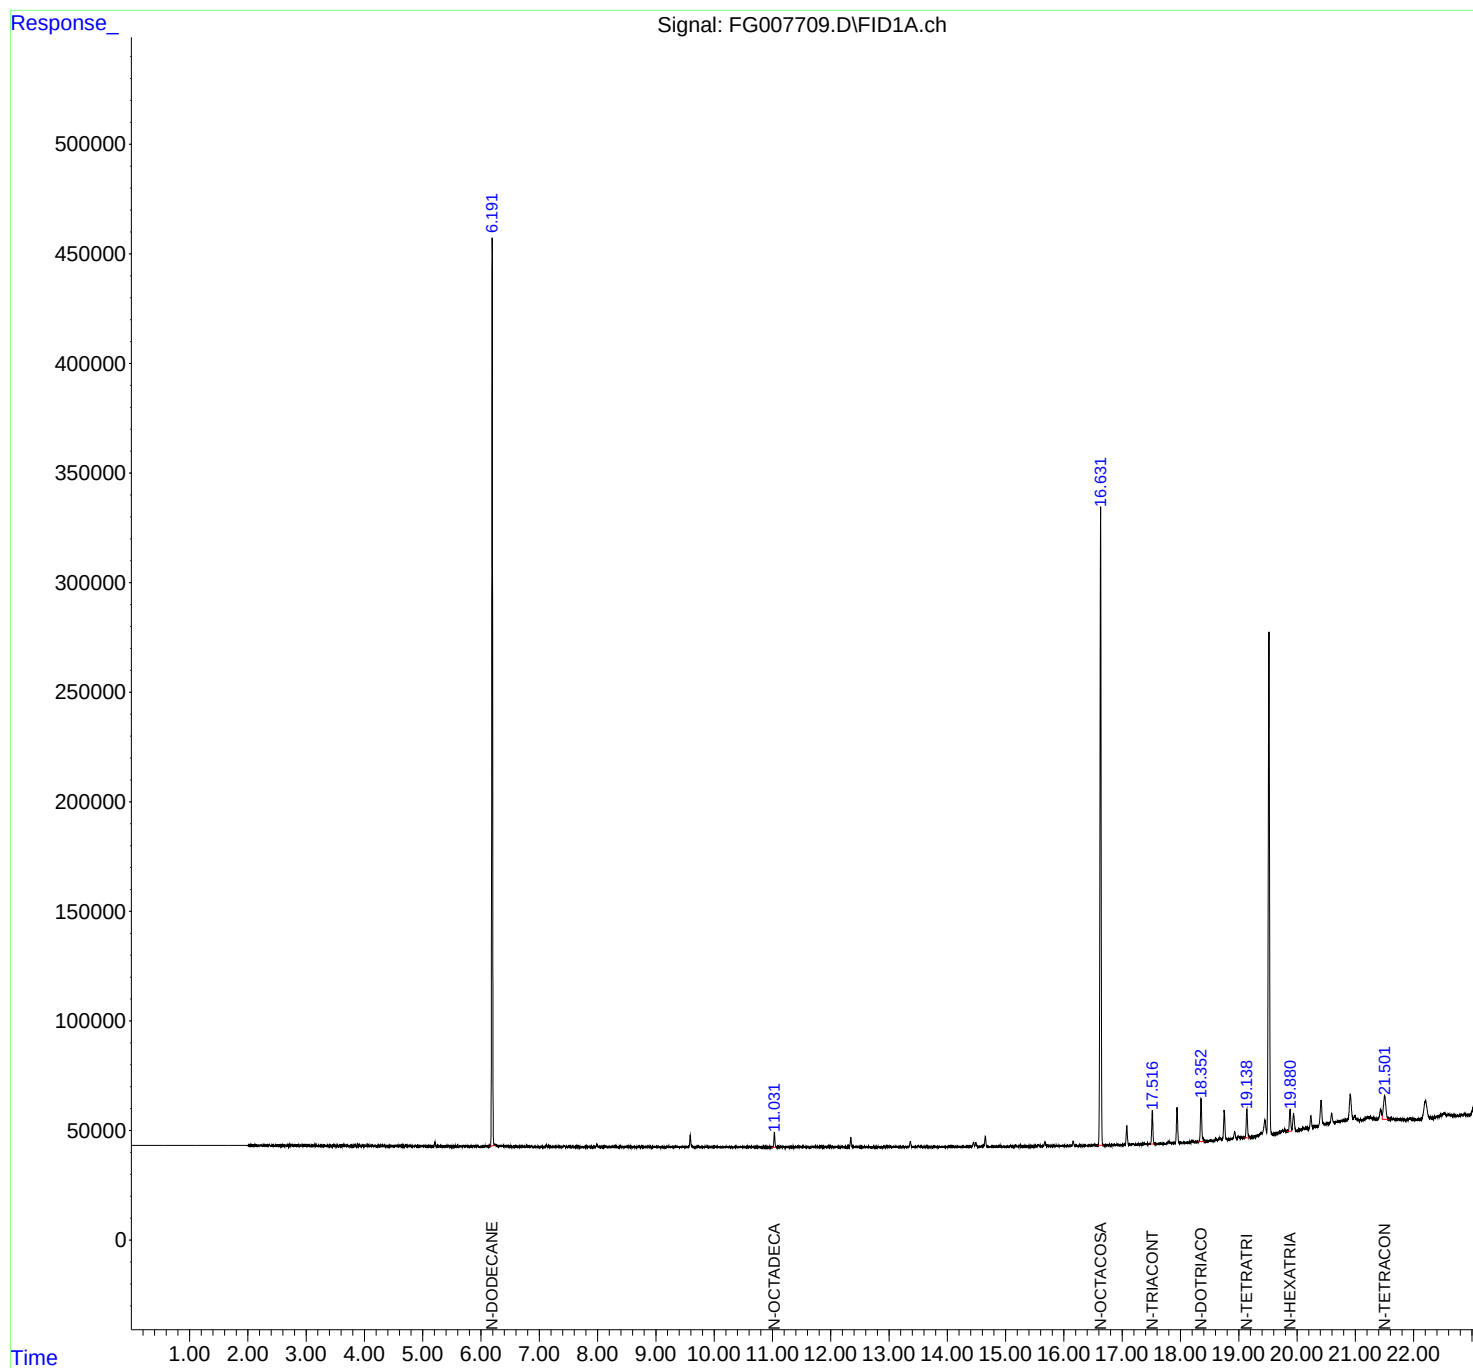


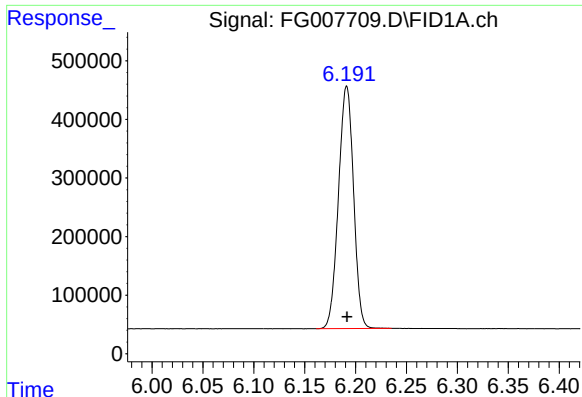

#3 N-DODECANE


R.T.: 6.191 min
Delta R.T.: 0.000 min
Response: 4269912
Conc: 28.83 ug/ml

Instrument :
FID_G
ClientSampleId :

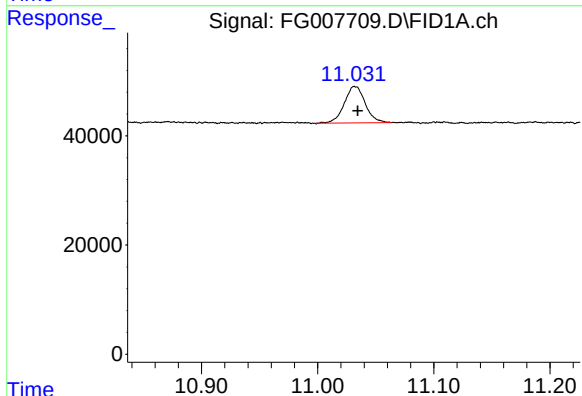


#6 N-OCTADECANE

R.T.: 11.032 min
Delta R.T.: -0.002 min
Response: 83332
Conc: 0.55 ug/ml

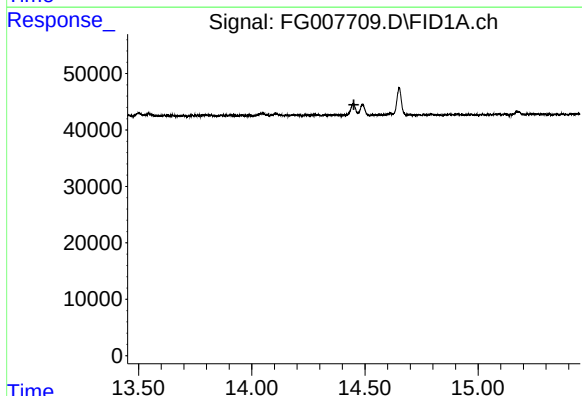


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.451 min
Response: 0
Conc: N.D.

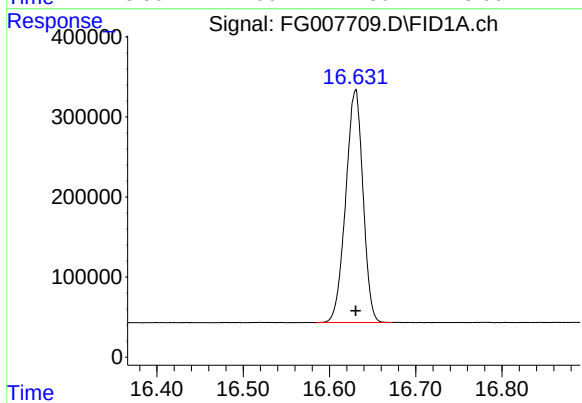

#12 N-OCTACOSANE


R.T.: 16.630 min
Delta R.T.: 0.000 min
Response: 4047792
Conc: 29.60 ug/ml

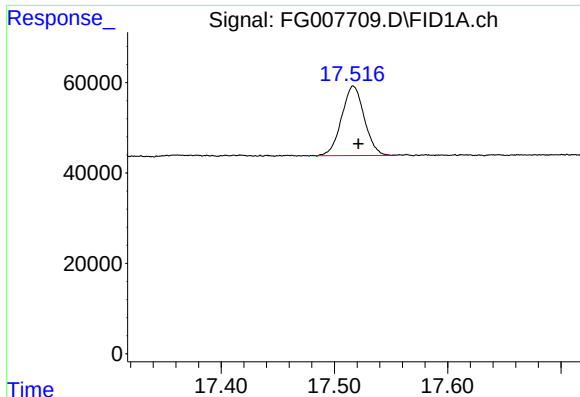

#13 N-TRIACONTANE


R.T.: 17.517 min
Delta R.T.: -0.004 min
Response: 213801
Conc: 1.62 ug/ml

Instrument :
FID_G
ClientSampleId :

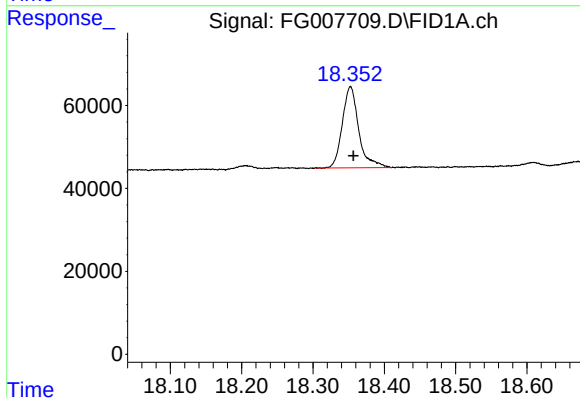


#14 N-DOTRIACONTANE

R.T.: 18.353 min
Delta R.T.: -0.004 min
Response: 313596
Conc: 2.49 ug/ml

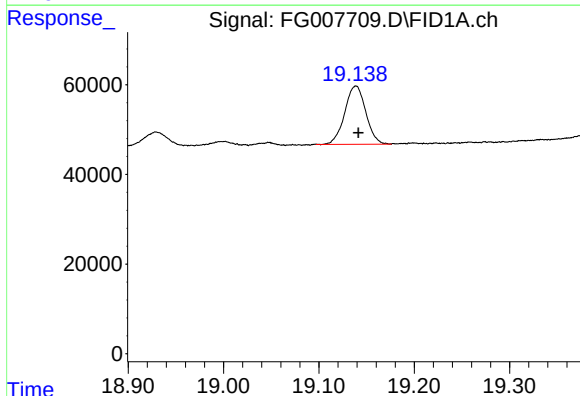


#15 N-TETRATRIACONTANE

R.T.: 19.139 min
Delta R.T.: -0.003 min
Response: 200268
Conc: 1.74 ug/ml

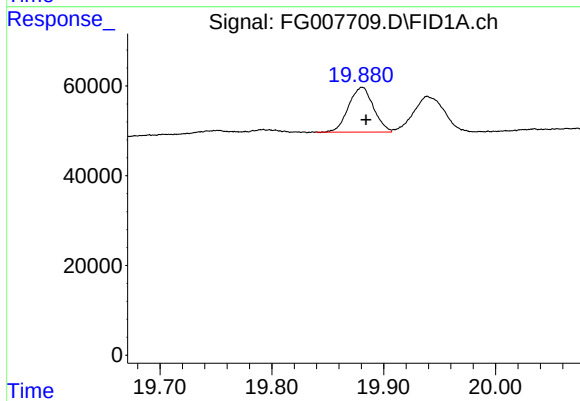

#16 N-HEXATRIACONTANE

R.T.: 19.881 min
Delta R.T.: -0.003 min
Response: 154915
Conc: 1.53 ug/ml

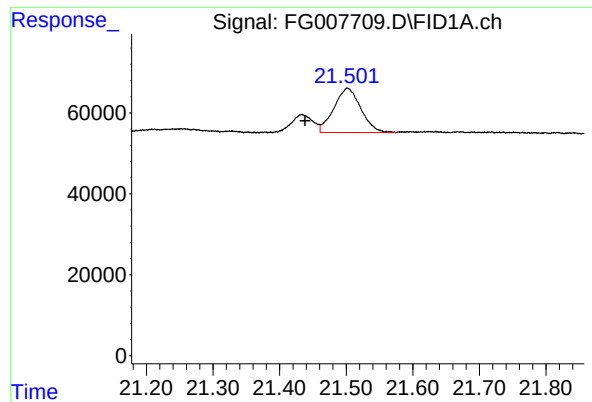

#18 N-TETRACONTANE

R.T.: 21.502 min
Delta R.T.: 0.064 min
Response: 306785
Conc: 3.50 ug/ml

Instrument :
FID_G
ClientSampleId :