

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031919\
Data File : FG004272.D
Signal(s) : FID1A.ch
Acq On : 19 Mar 2019 14:22
Operator : AJ\SJ
Sample : PB118046BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB118046BL

Integration File: autoint1.e
Quant Time: Mar 19 22:56:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.435	2002710	15.930 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031919\
Data File : FG004272.D
Signal(s) : FID1A.ch
Acq On : 19 Mar 2019 14:22
Operator : AJ\SJ
Sample : PB118046BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB118046BL

Integration File: autoint1.e
Quant Time: Mar 19 22:56:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

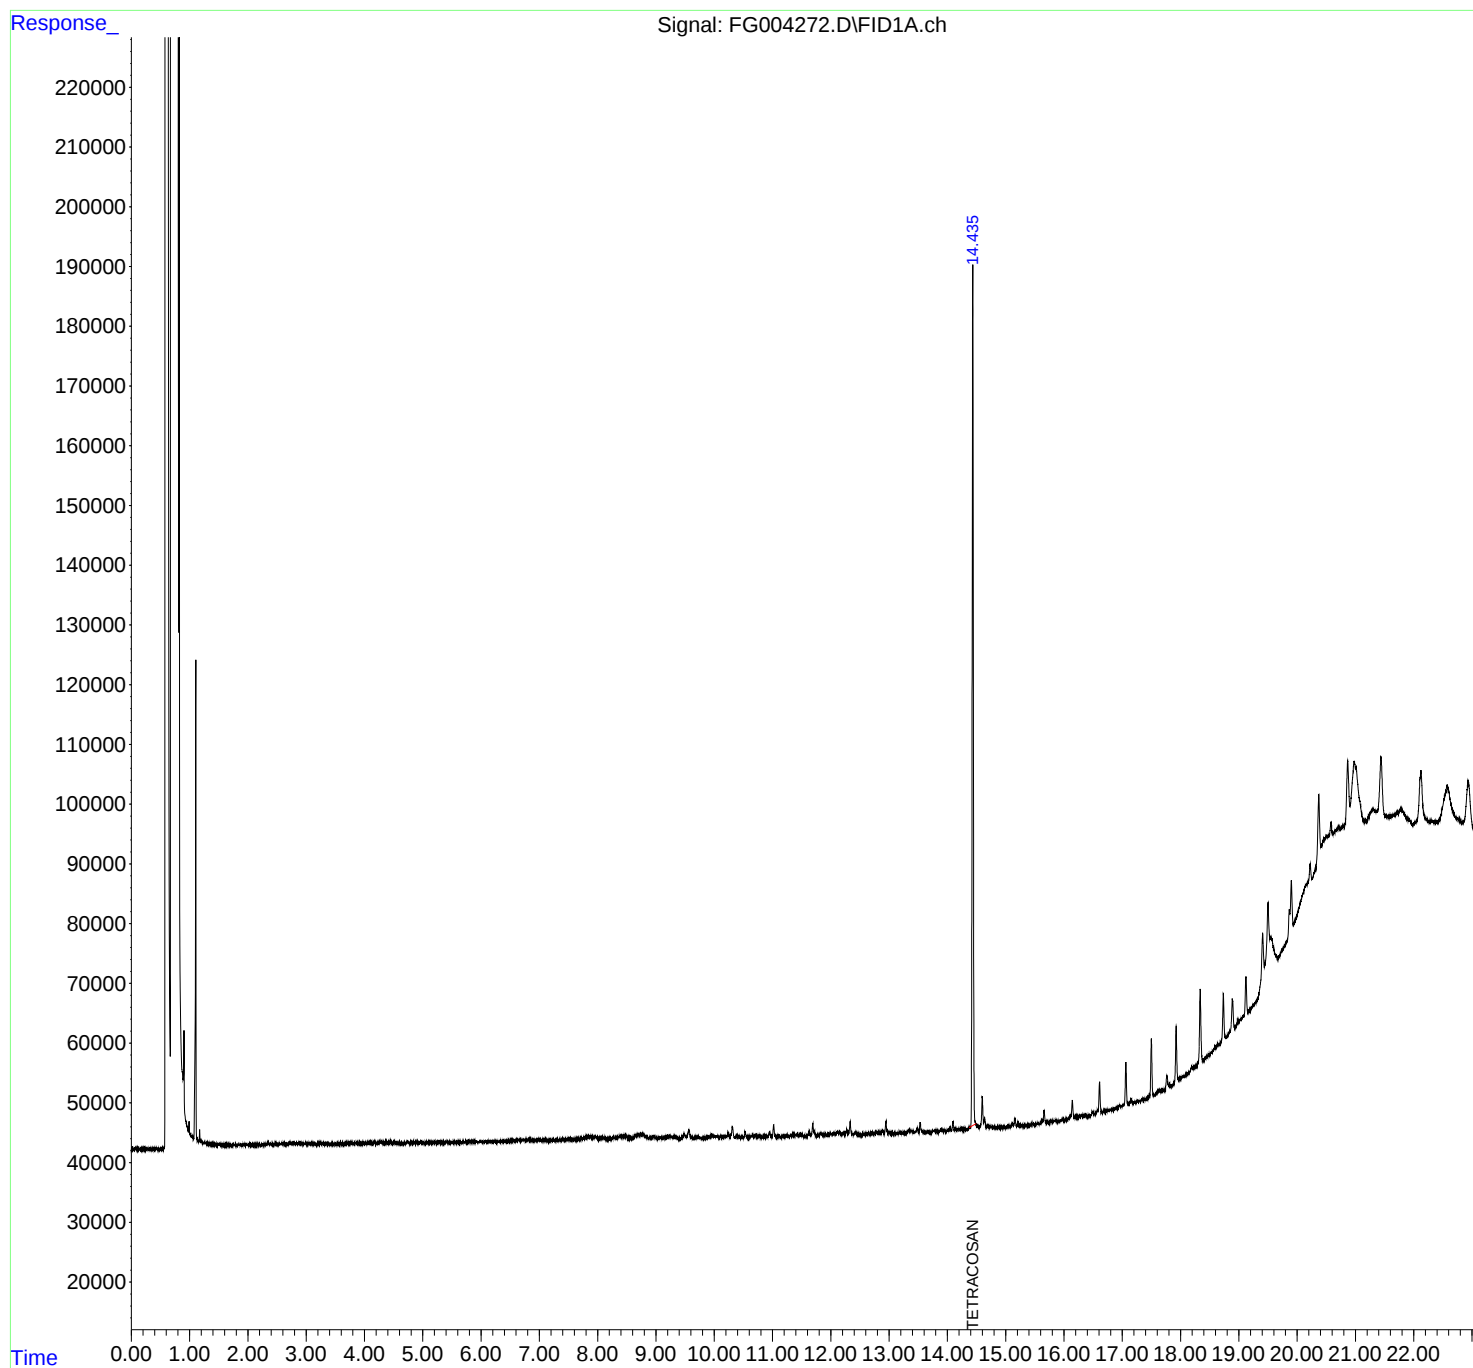

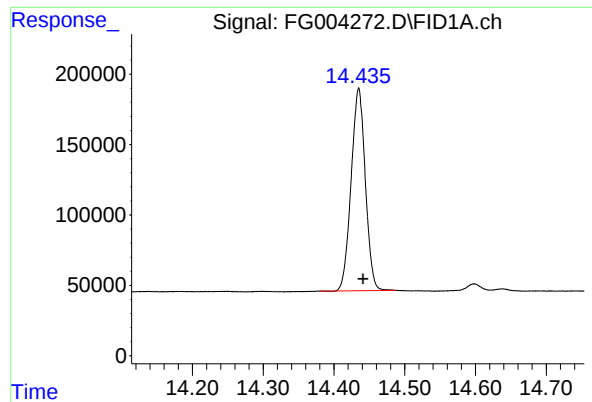

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.435 min
Delta R.T.: -0.006 min
Response: 2002710
Conc: 15.93 ug/ml

Instrument :
FID_G
ClientSampleId :
PB118046BL