

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031919\
Data File : FG004274.D
Signal(s) : FID1A.ch
Acq On : 19 Mar 2019 16:32
Operator : AJ\SJ
Sample : K1692-03 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
OK-02-031819

Integration File: autoint1.e
Quant Time: Mar 19 22:56:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
7) N-EICOSANE	12.380	1493251	10.453 ug/ml
8) N-DOCOSANE	13.546	221471	1.560 ug/ml
10) N-TETRACOSANE	14.607	945227	6.702 ug/ml
12) N-OCTACOSANE	16.617	292317	2.135 ug/ml
14) N-DOTRIACONTANE	18.335	412265	3.258 ug/ml
15) N-TETRATRIACONTANE	19.122	86429	0.729 ug/ml
16) N-HEXATRIACONTANE	19.899	506938	4.579 ug/ml
18) N-TETRACONTANE	21.438	820340	7.734 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031919\
Data File : FG004274.D
Signal(s) : FID1A.ch
Acq On : 19 Mar 2019 16:32
Operator : AJ\SJ
Sample : K1692-03 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :
OK-02-031819

Integration File: autoint1.e
Quant Time: Mar 19 22:56:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

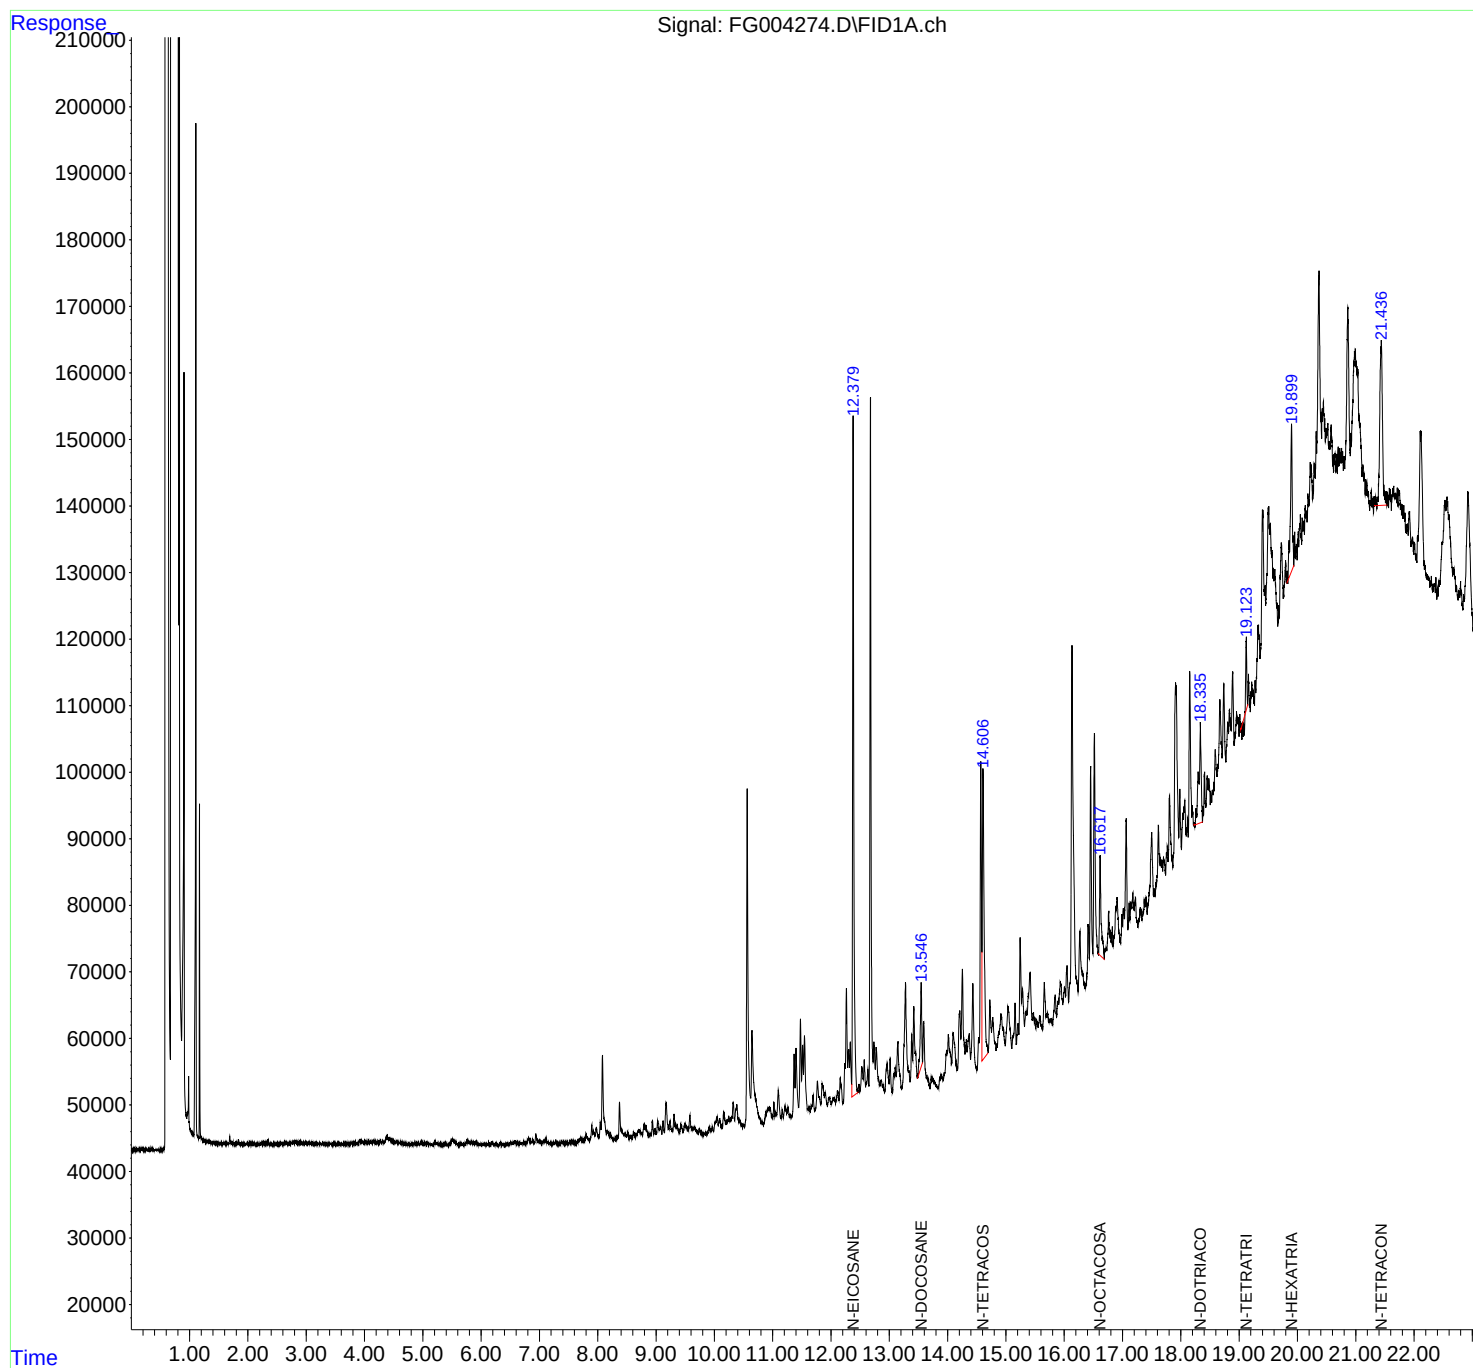


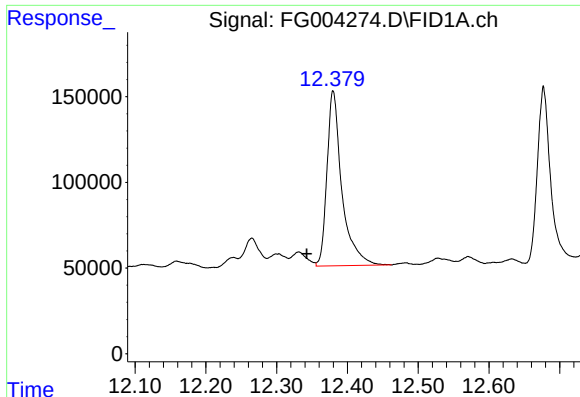

#7 N-EICOSANE


R.T.: 12.380 min
Delta R.T.: 0.037 min
Response: 1493251
Conc: 10.45 ug/ml

Instrument :
FID_G
ClientSampleId :
OK-02-031819

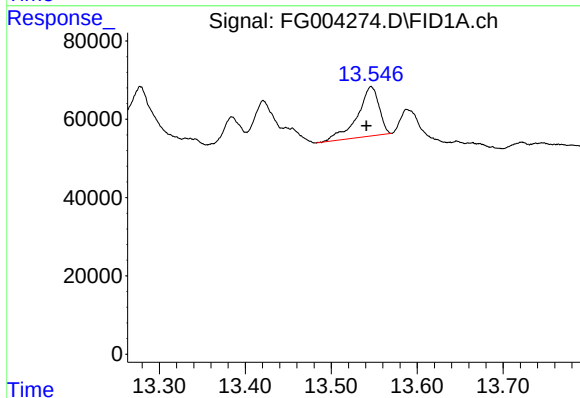


#8 N-DOCOSANE

R.T.: 13.546 min
Delta R.T.: 0.005 min
Response: 221471
Conc: 1.56 ug/ml

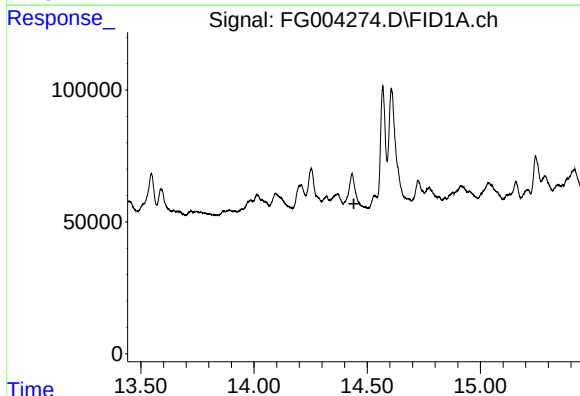


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.441 min
Response: 0
Conc: N.D.

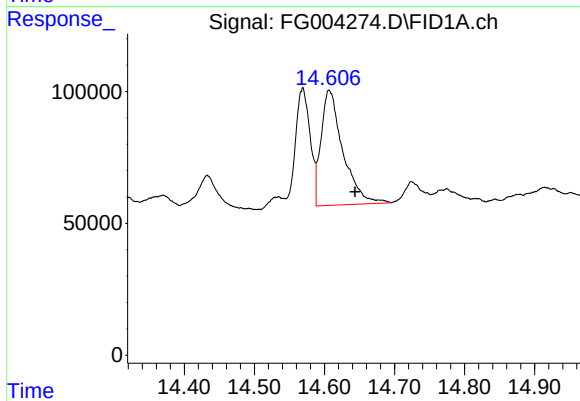

#10 N-TETRACOSANE


R.T.: 14.607 min
Delta R.T.: -0.037 min
Response: 945227
Conc: 6.70 ug/ml

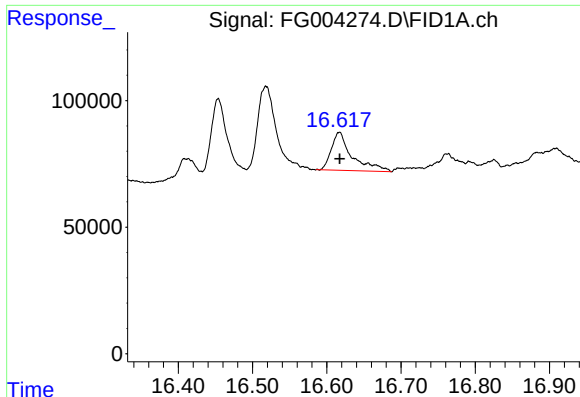

#12 N-OCTACOSANE


R.T.: 16.617 min
Delta R.T.: 0.000 min
Response: 292317
Conc: 2.14 ug/ml

Instrument :
FID_G
ClientSampleId :
OK-02-031819

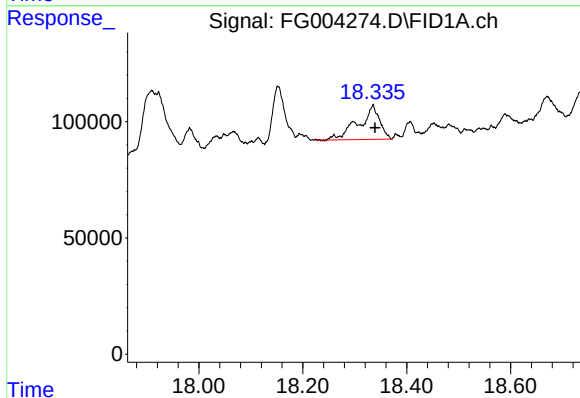


#14 N-DOTRIACONTANE

R.T.: 18.335 min
Delta R.T.: -0.004 min
Response: 412265
Conc: 3.26 ug/ml

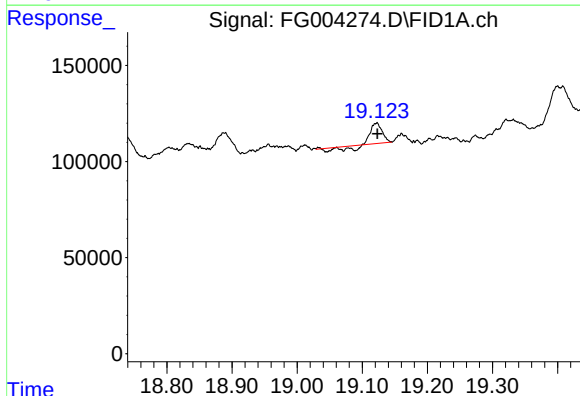


#15 N-TETRATRIACONTANE

R.T.: 19.122 min
Delta R.T.: -0.002 min
Response: 86429
Conc: 0.73 ug/ml

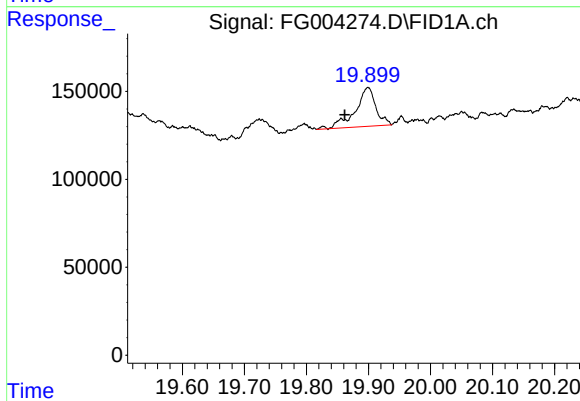

#16 N-HEXATRIACONTANE

R.T.: 19.899 min
Delta R.T.: 0.037 min
Response: 506938
Conc: 4.58 ug/ml

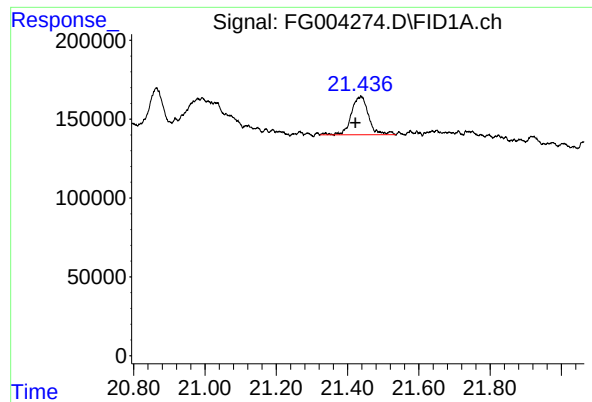

#18 N-TETRACONTANE

R.T.: 21.438 min
Delta R.T.: 0.016 min
Response: 820340
Conc: 7.73 ug/ml

Instrument :
FID_G
ClientSampleId :
OK-02-031819