

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031919\
 Data File : FG004275.D
 Signal(s) : FID1A.ch
 Acq On : 19 Mar 2019 17:03
 Operator : AJ\SJ
 Sample : K1956-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 TP-7-A

Integration File: autoint1.e
 Quant Time: Mar 19 22:56:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
 Quant Title :
 QLast Update : Tue Mar 05 03:05:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.433	1776449	14.130 ug/ml
Target Compounds			
4) N-TETRADECANE	8.039	432292	3.100 ug/ml
11) N-HEXACOSANE	15.658	730444	5.245 ug/ml
12) N-OCTACOSANE	16.610	1971338	14.399 ug/ml
13) N-TRIACONTANE	17.499	2136654	15.999 ug/ml
14) N-DOTRIACONTANE	18.332	1033543	8.168 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031919\
Data File : FG004275.D
Signal(s) : FID1A.ch
Acq On : 19 Mar 2019 17:03
Operator : AJ\SJ
Sample : K1956-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
TP-7-A

Integration File: autoint1.e
Quant Time: Mar 19 22:56:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

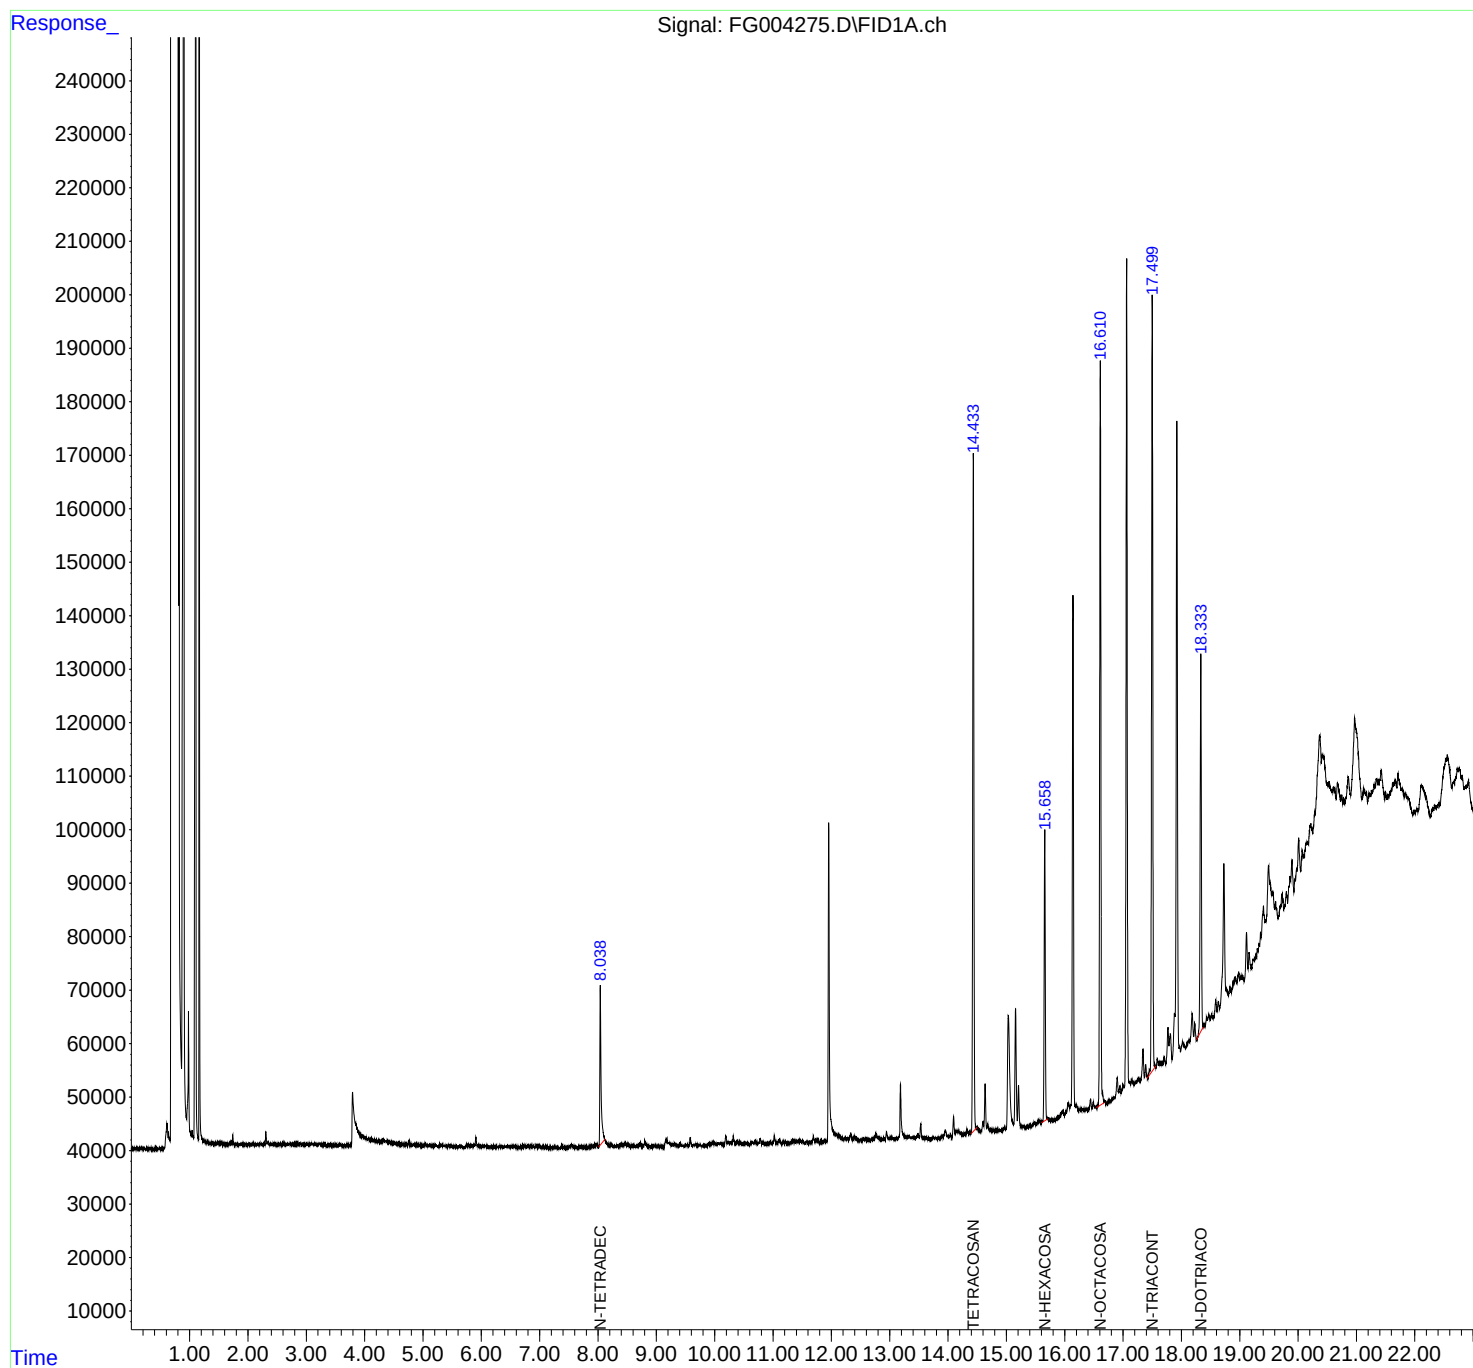


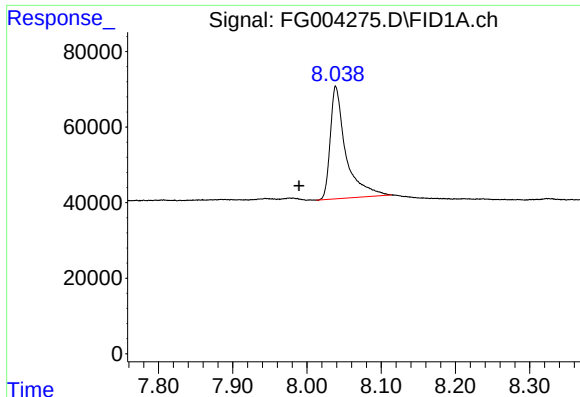

#4 N-TETRADECANE


R.T.: 8.039 min
Delta R.T.: 0.050 min
Response: 432292
Conc: 3.10 ug/ml

Instrument :
FID_G
ClientSampleId :
TP-7-A

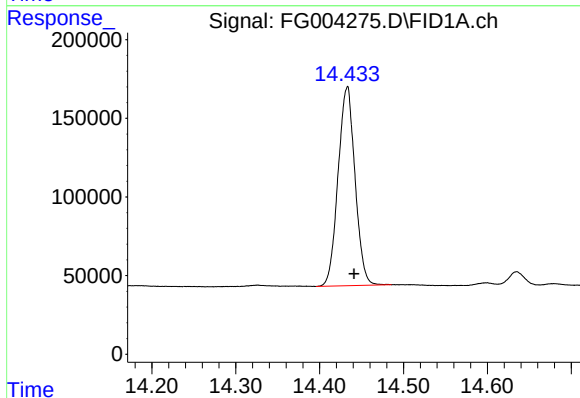


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.433 min
Delta R.T.: -0.008 min
Response: 1776449
Conc: 14.13 ug/ml

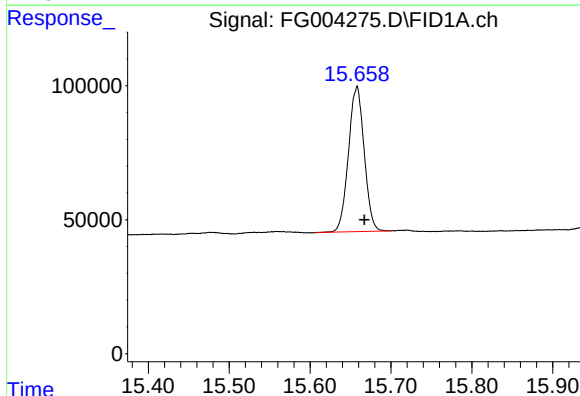


#11 N-HEXACOSANE

R.T.: 15.658 min
Delta R.T.: -0.009 min
Response: 730444
Conc: 5.24 ug/ml

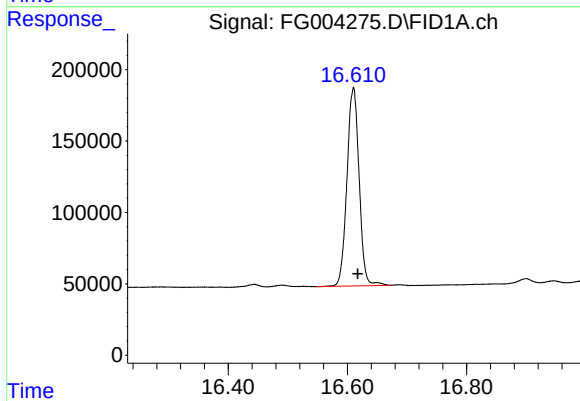

#12 N-OCTACOSANE


R.T.: 16.610 min
Delta R.T.: -0.008 min
Response: 1971338
Conc: 14.40 ug/ml

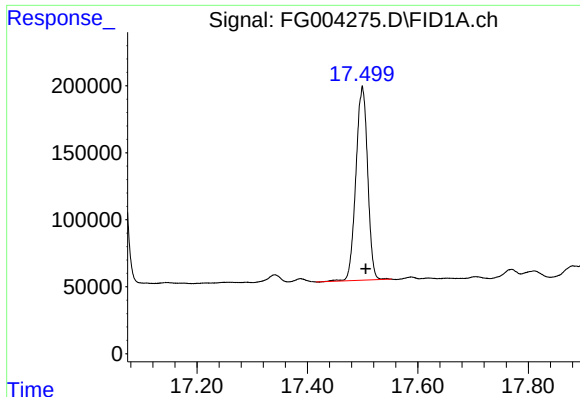

#13 N-TRIACONTANE

R.T.: 17.499 min
Delta R.T.: -0.006 min
Response: 2136654
Conc: 16.00 ug/ml

Instrument :
FID_G
ClientSampleId :
TP-7-A

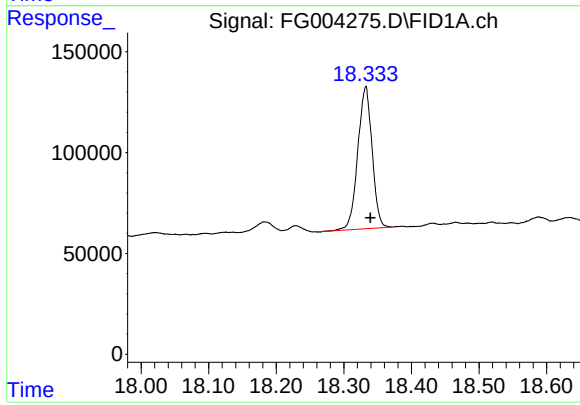

#14 N-DOTRIACONTANE

R.T.: 18.332 min
Delta R.T.: -0.007 min
Response: 1033543
Conc: 8.17 ug/ml