

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031919\
 Data File : FG004277.D
 Signal(s) : FID1A.ch
 Acq On : 19 Mar 2019 18:03
 Operator : AJ\SJ
 Sample : K1956-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 TP-8-B

Integration File: autoint1.e
 Quant Time: Mar 19 22:57:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
 Quant Title :
 QLast Update : Tue Mar 05 03:05:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.433	2161573	17.194 ug/ml
Target Compounds			
4) N-TETRADECANE	8.037	1222941	8.770 ug/ml
10) N-TETRACOSANE	14.635	181225	1.285 ug/ml
11) N-HEXACOSANE	15.657	978242	7.024 ug/ml
12) N-OCTACOSANE	16.609	2589243	18.912 ug/ml
13) N-TRIACONTANE	17.499	2878822	21.557 ug/ml
14) N-DOTRIACONTANE	18.331	1540789	12.177 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031919\
Data File : FG004277.D
Signal(s) : FID1A.ch
Acq On : 19 Mar 2019 18:03
Operator : AJ\SJ
Sample : K1956-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
TP-8-B

Integration File: autoint1.e
Quant Time: Mar 19 22:57:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

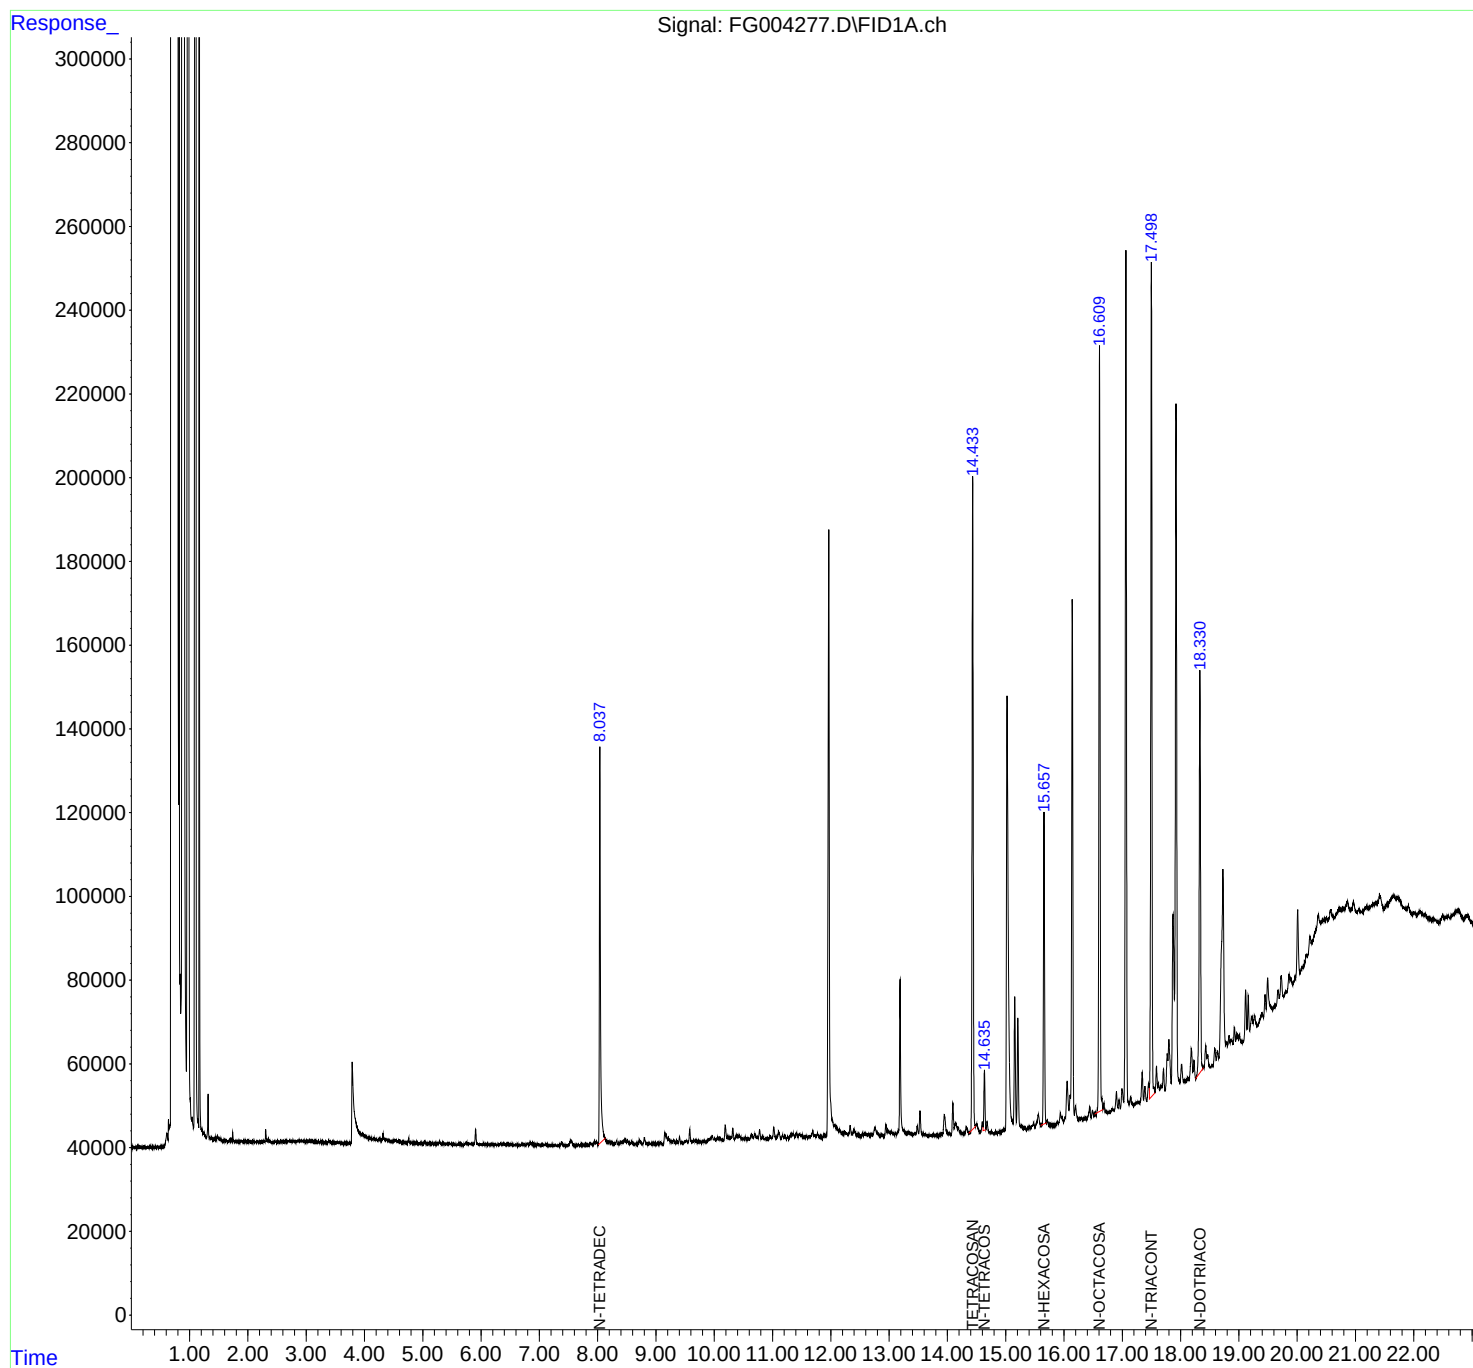


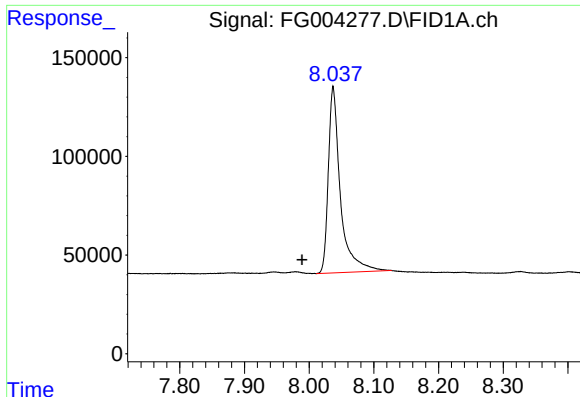

#4 N-TETRADECANE


R.T.: 8.037 min
Delta R.T.: 0.048 min
Response: 1222941
Conc: 8.77 ug/ml

Instrument :
FID_G
ClientSampleId :
TP-8-B

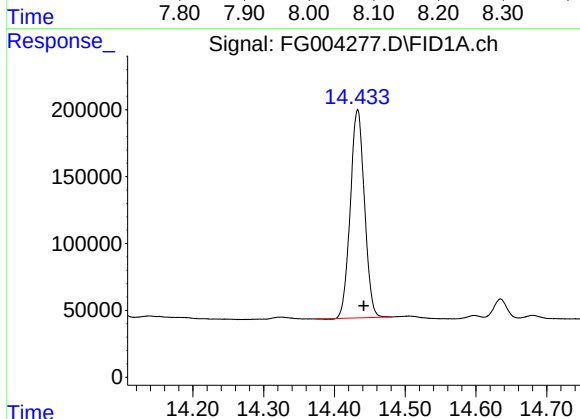


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.433 min
Delta R.T.: -0.008 min
Response: 2161573
Conc: 17.19 ug/ml

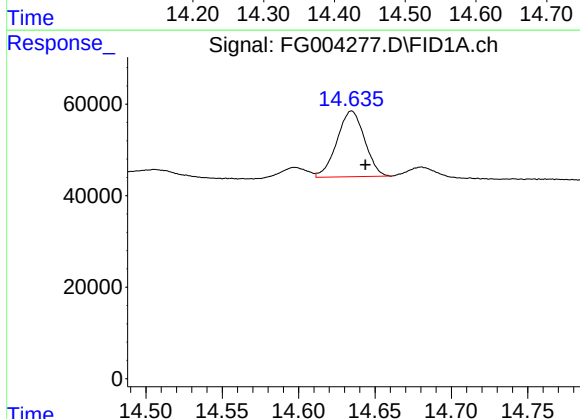


#10 N-TETRACOSANE

R.T.: 14.635 min
Delta R.T.: -0.009 min
Response: 181225
Conc: 1.29 ug/ml

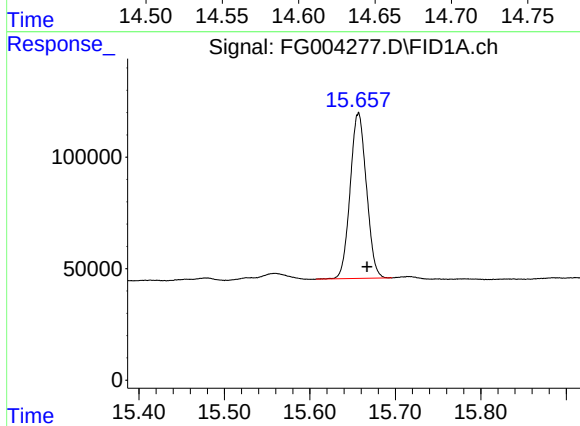

#11 N-HEXACOSANE


R.T.: 15.657 min
Delta R.T.: -0.010 min
Response: 978242
Conc: 7.02 ug/ml

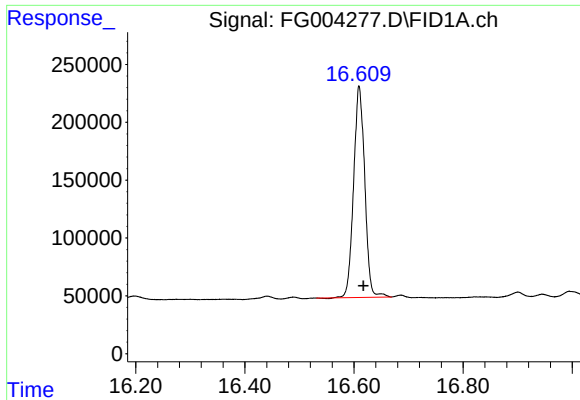

#12 N-OCTACOSANE


R.T.: 16.609 min
Delta R.T.: -0.008 min
Response: 2589243
Conc: 18.91 ug/ml

Instrument :
FID_G
ClientSampleId :
TP-8-B

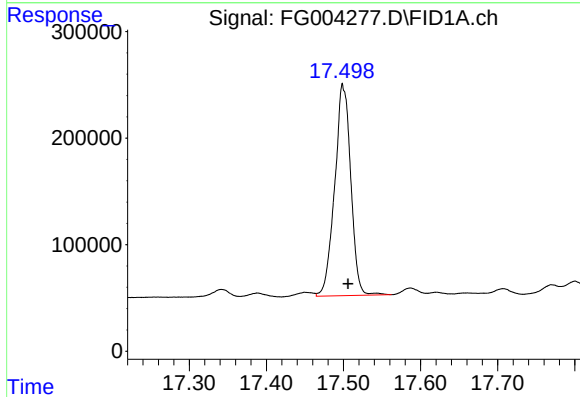

#13 N-TRIACONTANE

R.T.: 17.499 min
Delta R.T.: -0.007 min
Response: 2878822
Conc: 21.56 ug/ml

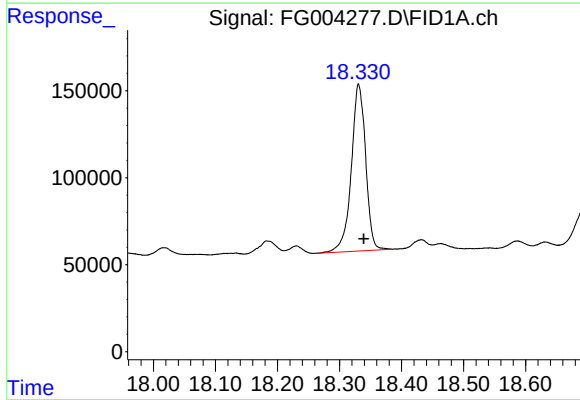

#14 N-DOTRIACONTANE

R.T.: 18.331 min
Delta R.T.: -0.008 min
Response: 1540789
Conc: 12.18 ug/ml