

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031919\
Data File : FG004271.D
Signal(s) : FID1A.ch
Acq On : 19 Mar 2019 12:10
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: Sample.e
Quant Time: Mar 19 22:56:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.183	2697735	19.900 ug/ml
12) N-OCTACOSANE	16.614	2546690	18.601 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031919\
Data File : FG004271.D
Signal(s) : FID1A.ch
Acq On : 19 Mar 2019 12:10
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: Sample.e
Quant Time: Mar 19 22:56:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

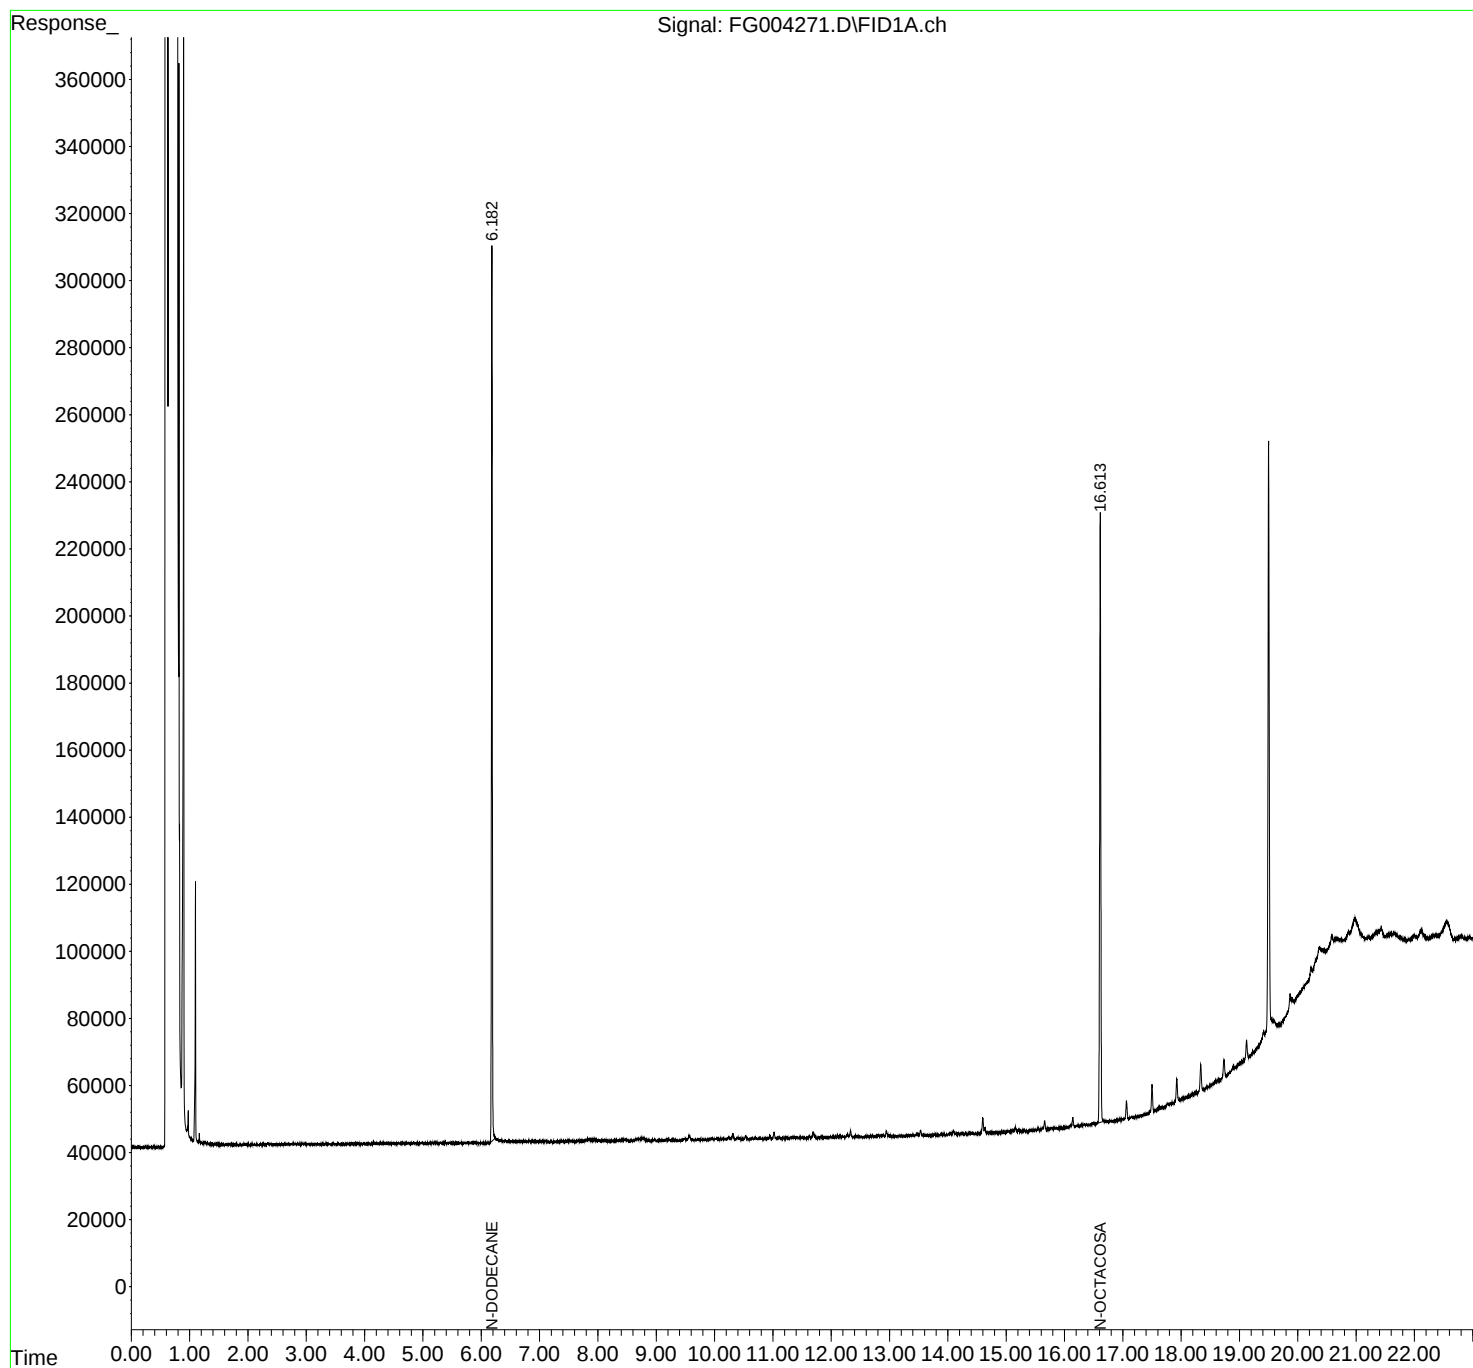


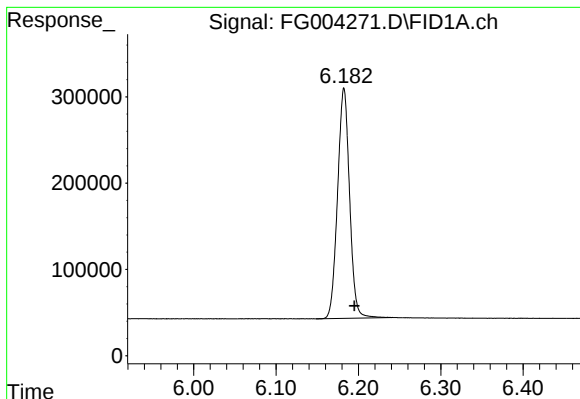

#3 N-DODECANE


R.T.: 6.183 min
Delta R.T.: -0.013 min
Response: 2697735
Conc: 19.90 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

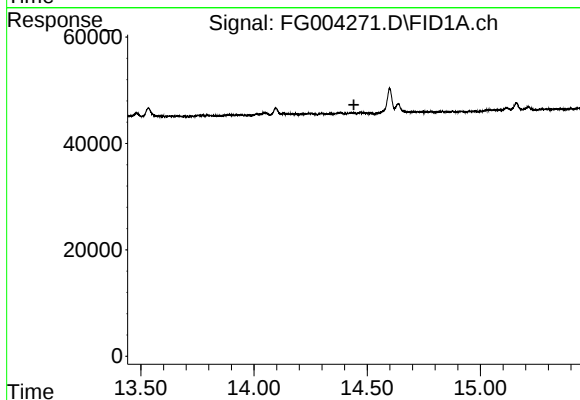

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.441 min
Response: 0
Conc: N.D.

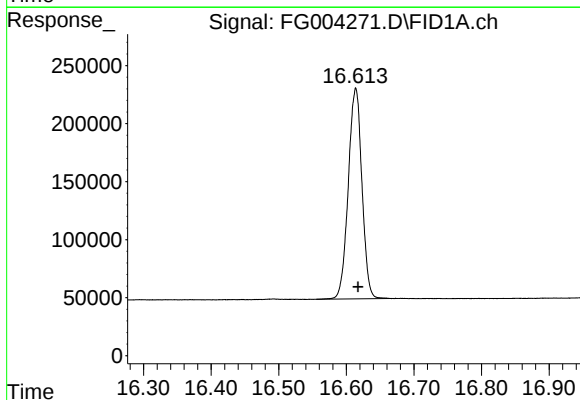

#12 N-OCTACOSANE

R.T.: 16.614 min
Delta R.T.: -0.004 min
Response: 2546690
Conc: 18.60 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

rteres

Area Percent Report

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031919\
Data File : FG004271.D
Signal(s) : FID1A.ch
Acq On : 19 Mar 2019 12:10
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Title :

Signal : FID1A.ch

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	6.183	6.149	6.240	BB	266921	2697735	100.00%	51.440%
2	16.614	16.555	16.667	BB	181741	2546690	94.40%	48.560%
Sum of corrected areas:						5244425		

FG030419.M Wed Mar 20 10:21:07 2019