

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031921\
Data File : FG007721.D
Signal(s) : FID1A.ch
Acq On : 19 Mar 2021 09:21
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 19 22:45:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031221.M
Quant Title :
QLast Update : Mon Mar 15 09:29:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.449	2637823	20.847 ug/ml
Target Compounds			
16) N-HEXATRIACONTANE	19.943f	263552	2.605 ug/ml
18) N-TETRACONTANE	21.506f	571756	6.529 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031921\
Data File : FG007721.D
Signal(s) : FID1A.ch
Acq On : 19 Mar 2021 09:21
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 19 22:45:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031221.M
Quant Title :
QLast Update : Mon Mar 15 09:29:28 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

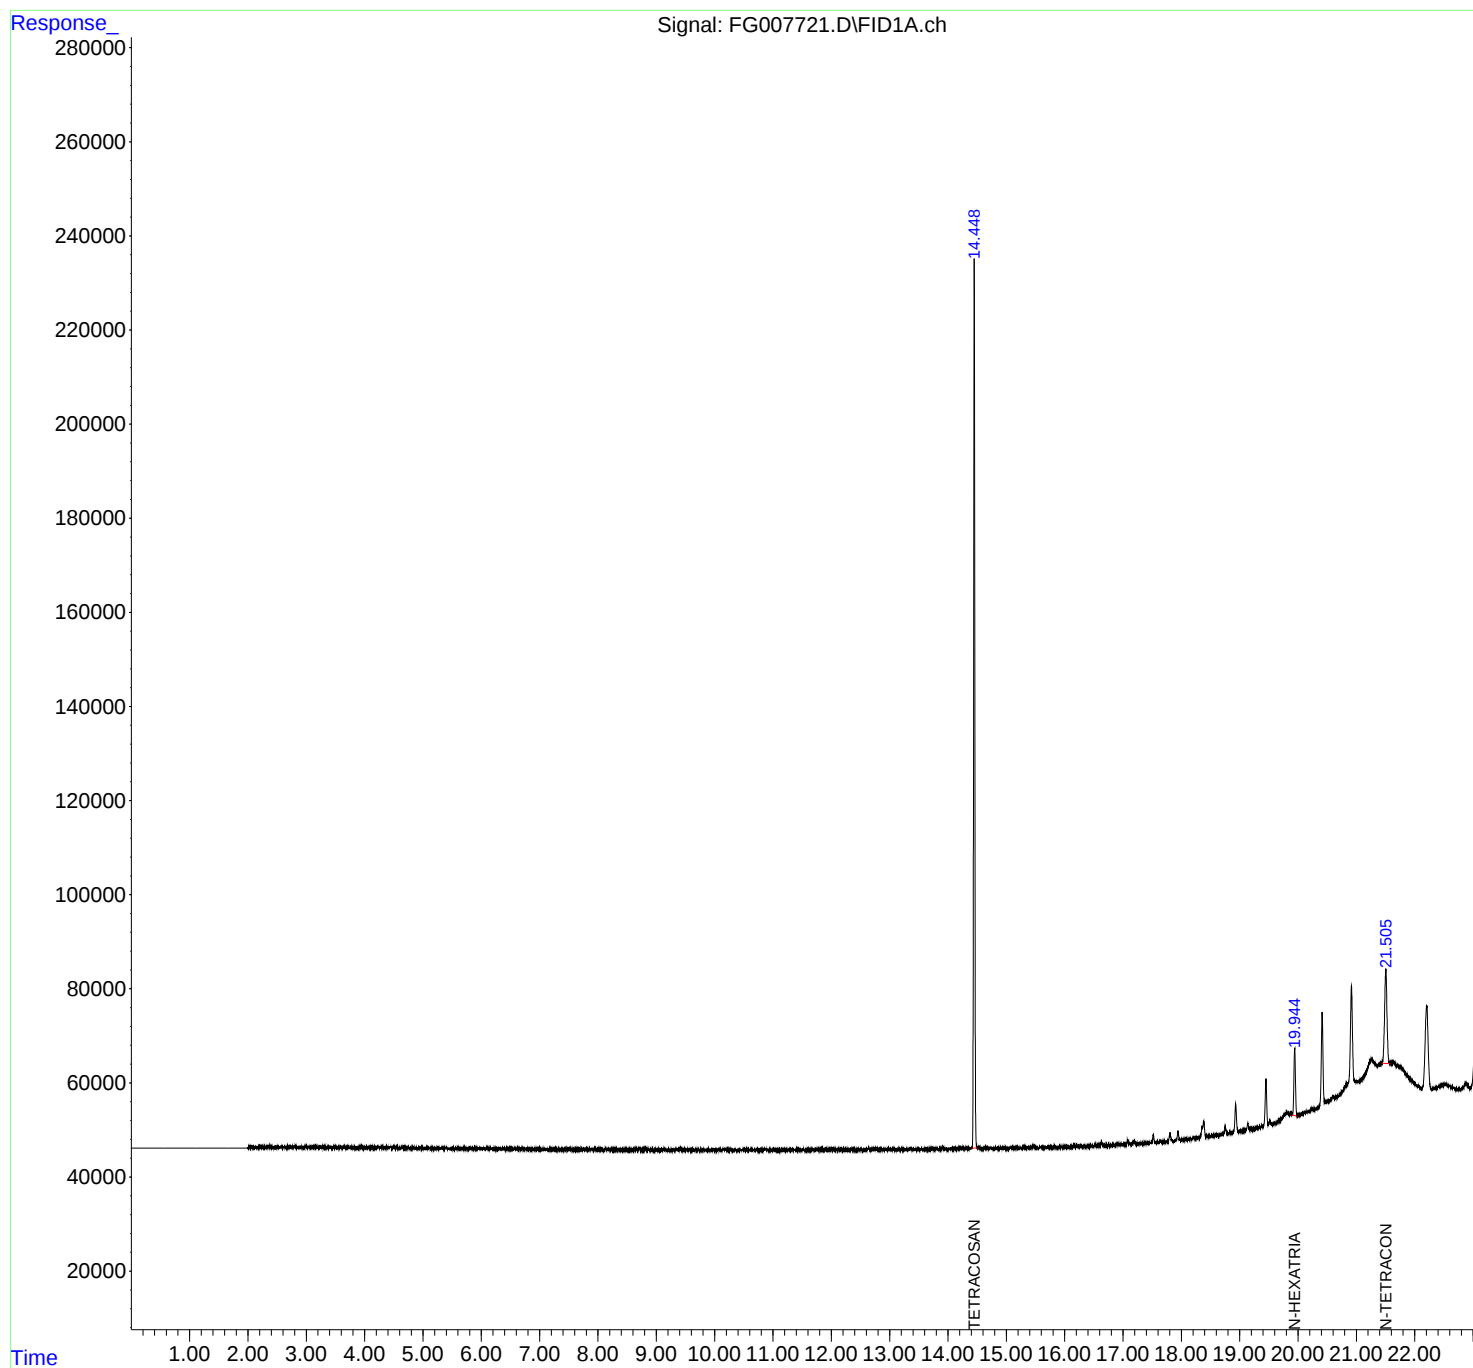

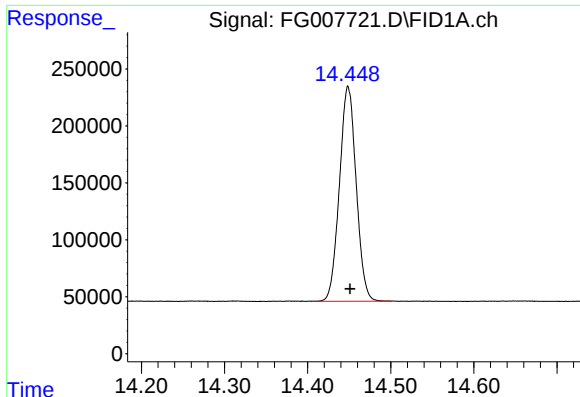


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.449 min
Delta R.T.: -0.003 min
Response: 2637823
Conc: 20.85 ug/ml

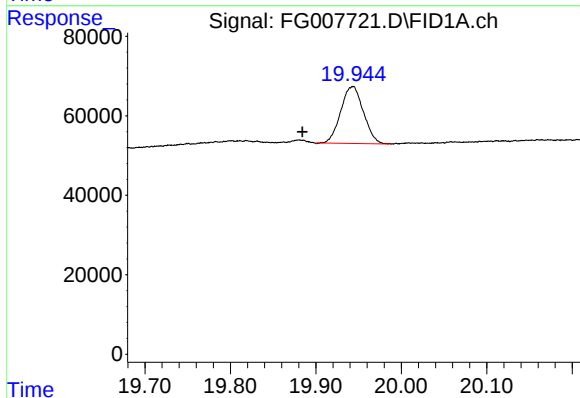

#16 N-HEXATRIACONTANE

R.T.: 19.943 min
Delta R.T.: 0.059 min
Response: 263552
Conc: 2.60 ug/ml

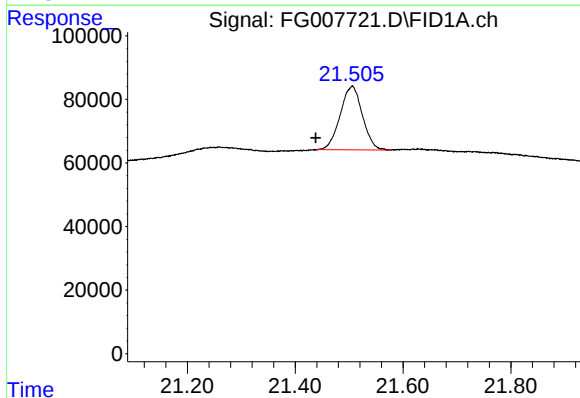

#18 N-TETRACONTANE

R.T.: 21.506 min
Delta R.T.: 0.068 min
Response: 571756
Conc: 6.53 ug/ml