

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032019\
Data File : FG004294.D
Signal(s) : FID1A.ch
Acq On : 20 Mar 2019 19:26
Operator : AJ\SJ
Sample : K1688-37 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 21 08:52:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.184	271257	2.001 ug/ml
4) N-TETRADECANE	7.978	266310	1.910 ug/ml
5) N-HEXADECANE	9.578	230011	1.616 ug/ml
6) N-OCTADECANE	11.019	161216	1.124 ug/ml
12) N-OCTACOSANE	16.607	160423	1.172 ug/ml
13) N-TRIACONTANE	17.499	258193	1.933 ug/ml
14) N-DOTRIACONTANE	18.331	305716	2.416 ug/ml
15) N-TETRATRIACONTANE	19.119	194311	1.640 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032019\
Data File : FG004294.D
Signal(s) : FID1A.ch
Acq On : 20 Mar 2019 19:26
Operator : AJ\SJ
Sample : K1688-37 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 21 08:52:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

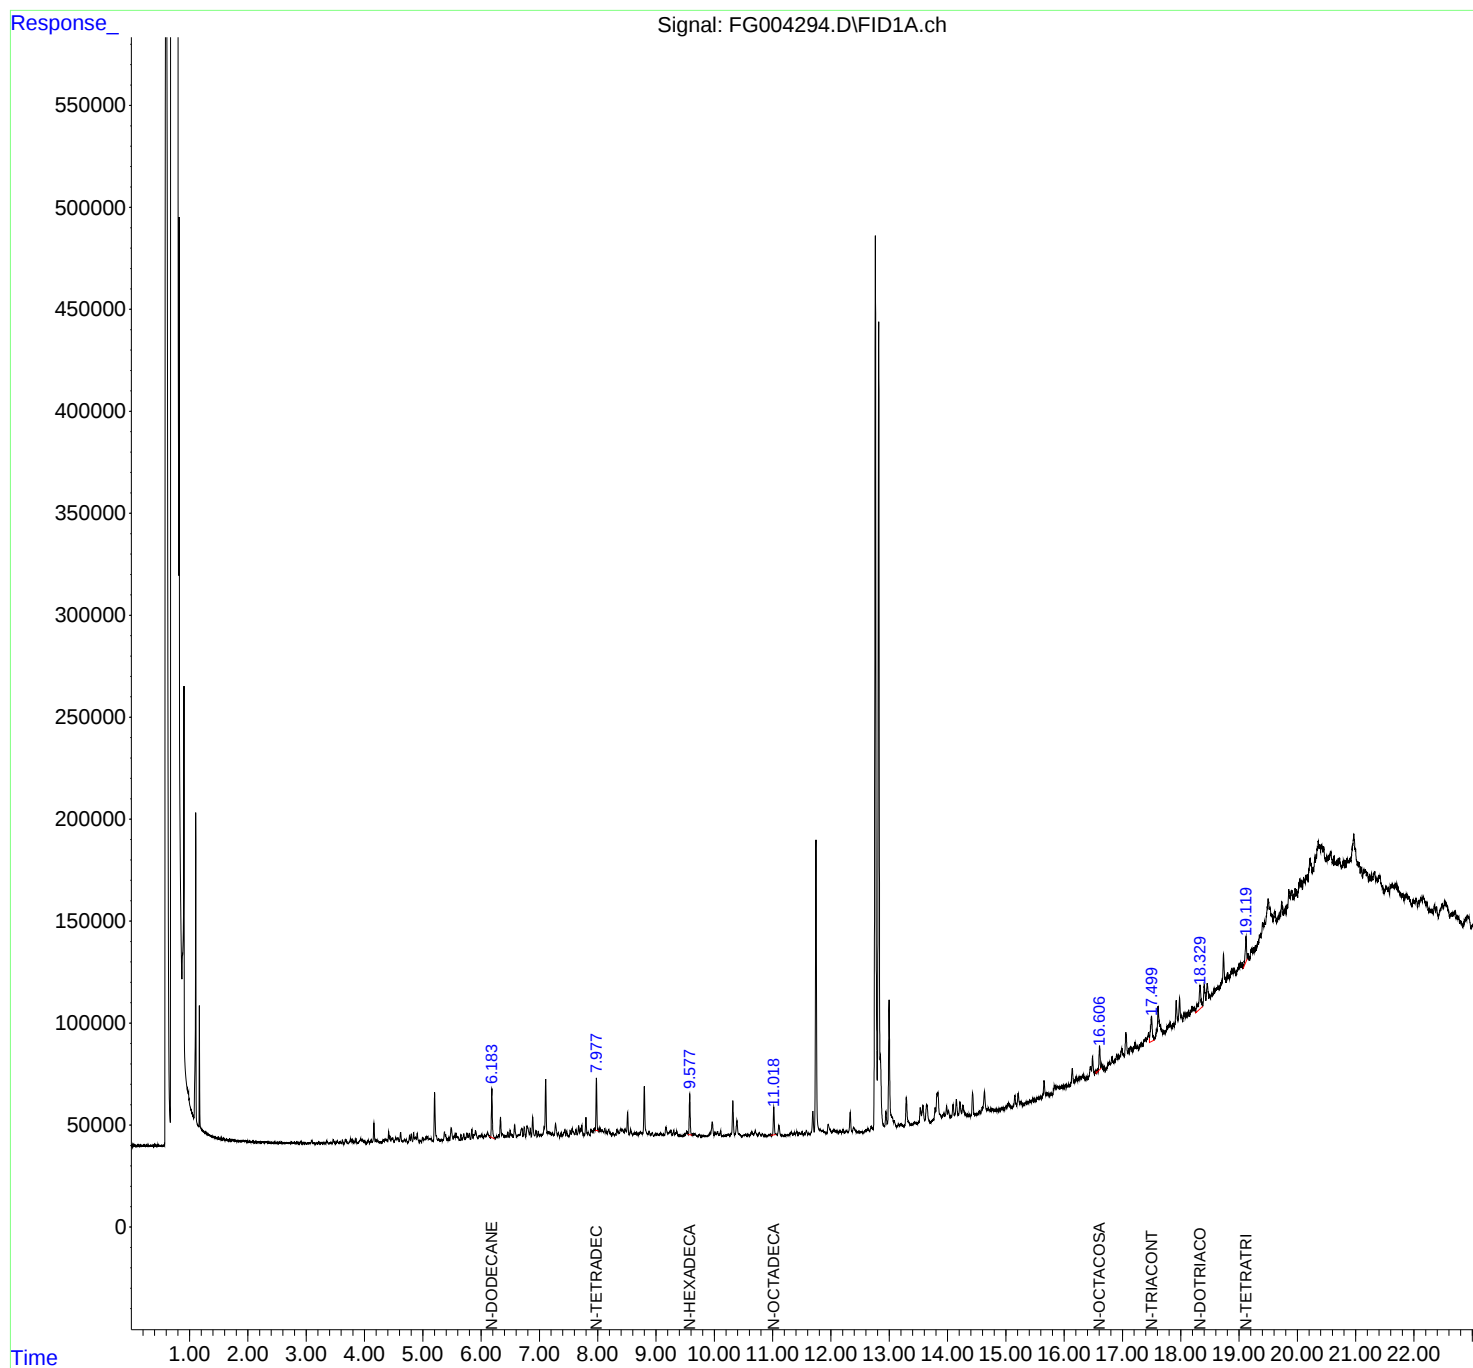

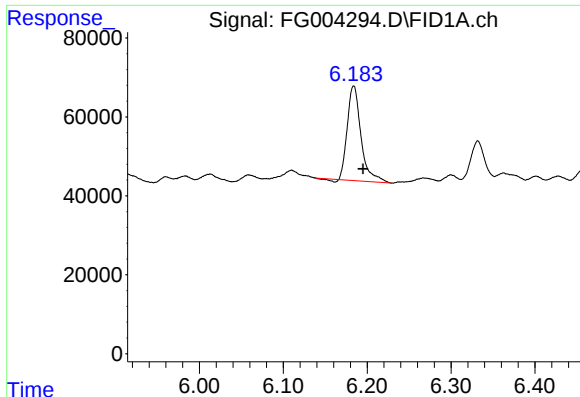


#3 N-DODECANE

R.T.: 6.184 min
Delta R.T.: -0.011 min
Response: 271257
Conc: 2.00 ug/ml

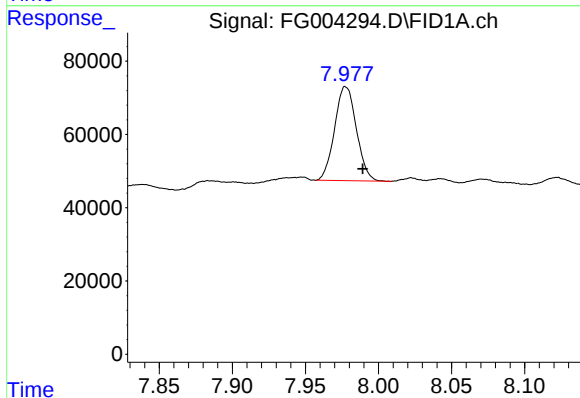


#4 N-TETRADECANE

R.T.: 7.978 min
Delta R.T.: -0.012 min
Response: 266310
Conc: 1.91 ug/ml

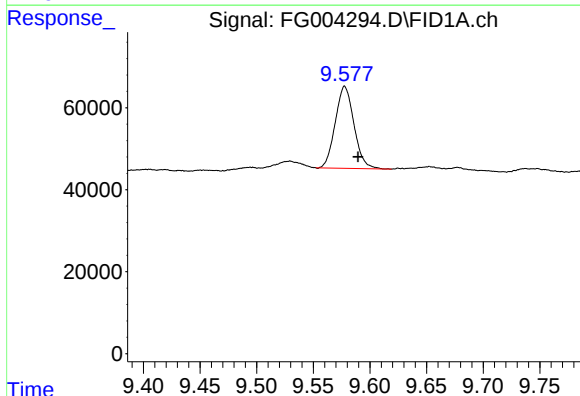


#5 N-HEXADECANE

R.T.: 9.578 min
Delta R.T.: -0.012 min
Response: 230011
Conc: 1.62 ug/ml

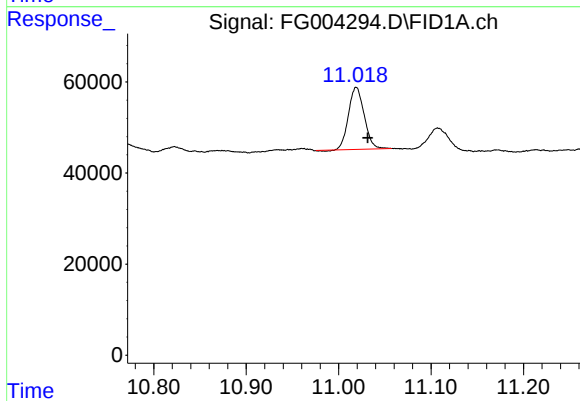


#6 N-OCTADECANE

R.T.: 11.019 min
Delta R.T.: -0.012 min
Response: 161216
Conc: 1.12 ug/ml

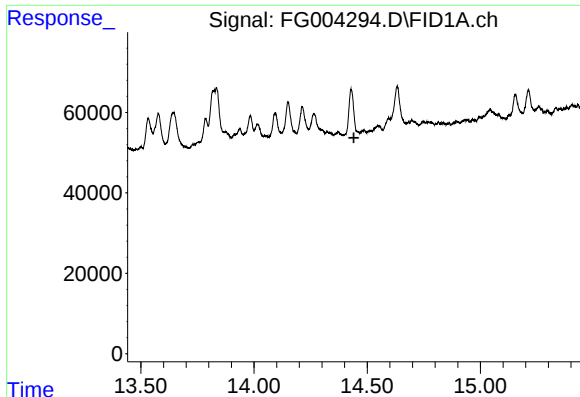


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.441 min
Response: 0
Conc: N.D.

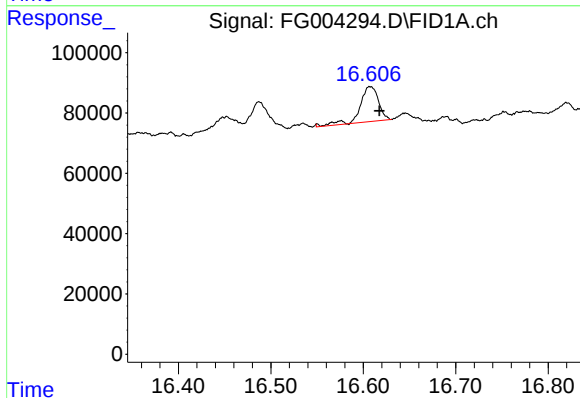


#12 N-OCTACOSANE

R.T.: 16.607 min
Delta R.T.: -0.010 min
Response: 160423
Conc: 1.17 ug/ml

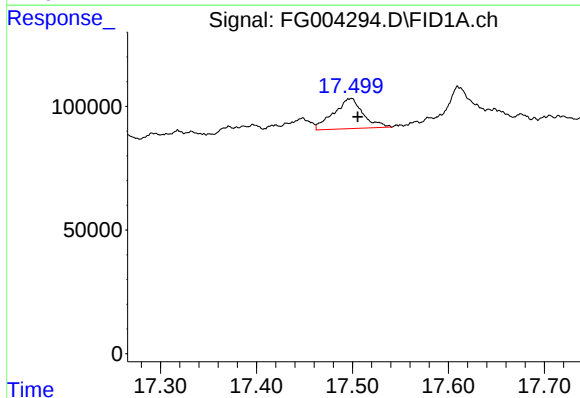


#13 N-TRIACONTANE

R.T.: 17.499 min
Delta R.T.: -0.007 min
Response: 258193
Conc: 1.93 ug/ml

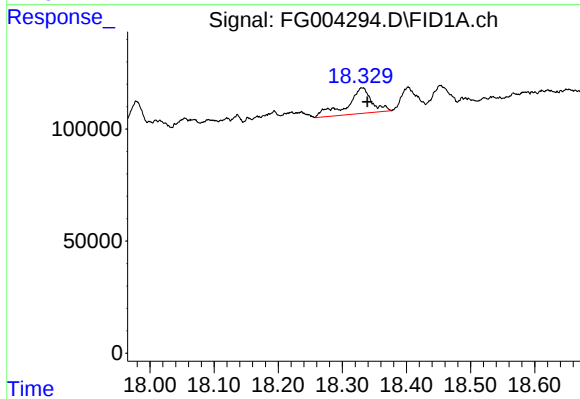

#14 N-DOTRIACONTANE

R.T.: 18.331 min
Delta R.T.: -0.008 min
Response: 305716
Conc: 2.42 ug/ml

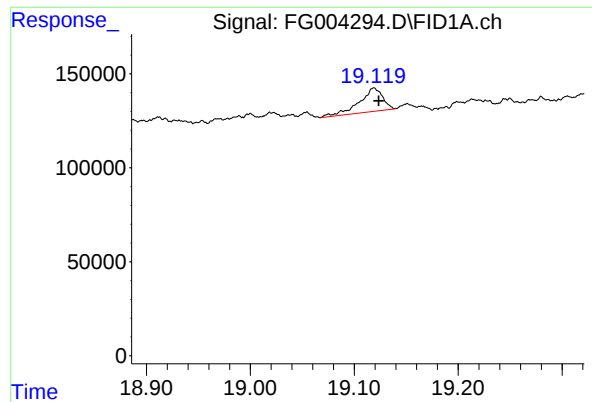

#15 N-TETRATRIACONTANE

R.T.: 19.119 min

Delta R.T.: -0.005 min

Response: 194311

Conc: 1.64 ug/ml