

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032023\
Data File : FG011631.D
Signal(s) : FID1A.ch
Acq On : 20 Mar 2023 17:37
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 21 04:16:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.054	2098825	20.852 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.958	50296	0.542 ug/ml
15) N-TETRATRIACONTANE	19.742	35620	0.423 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032023\
Data File : FG011631.D
Signal(s) : FID1A.ch
Acq On : 20 Mar 2023 17:37
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 21 04:16:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

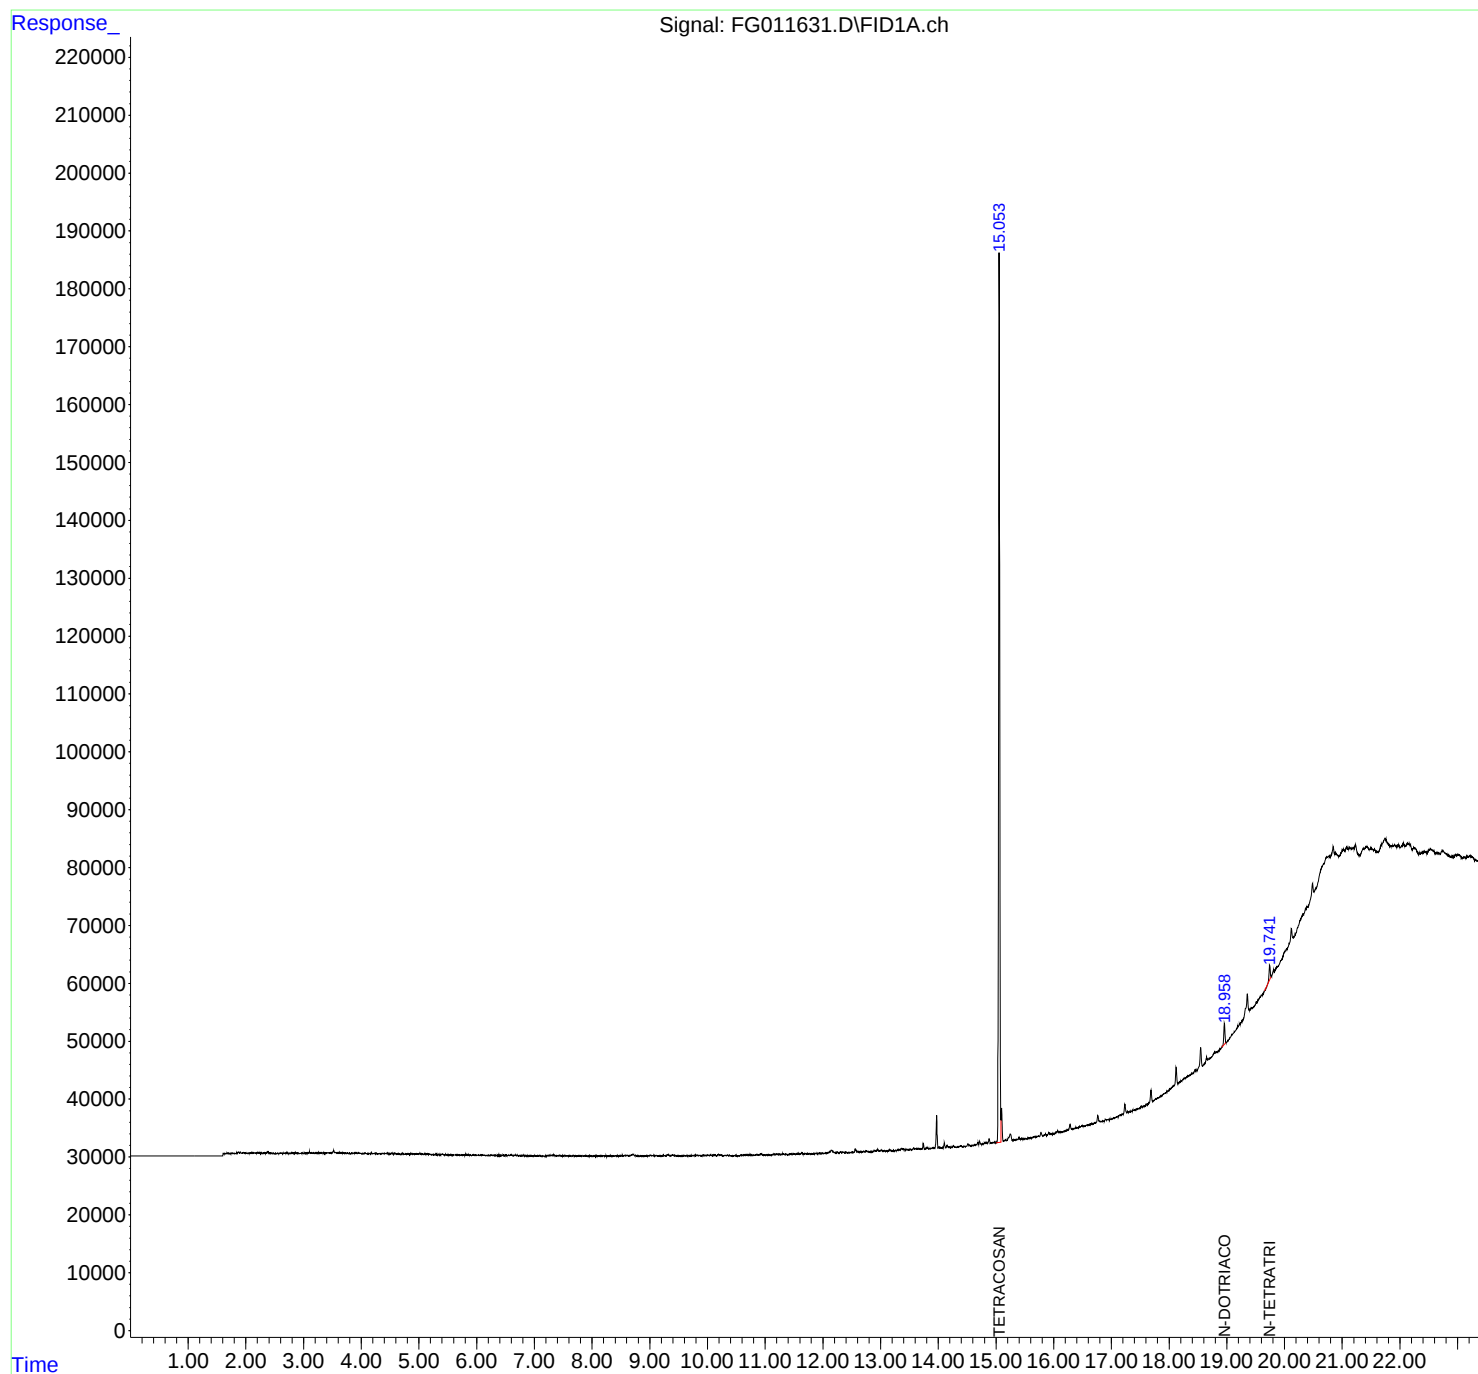

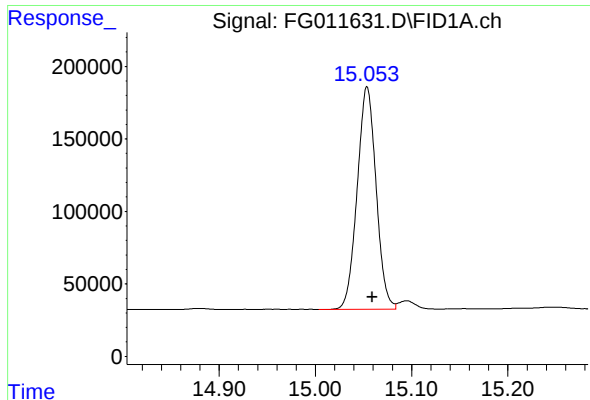


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.054 min
Delta R.T.: -0.005 min
Response: 2098825
Conc: 20.85 ug/ml

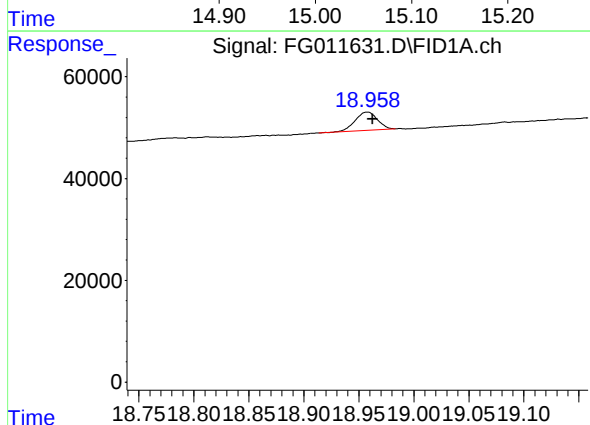

#14 N-DOTRIACONTANE

R.T.: 18.958 min
Delta R.T.: -0.005 min
Response: 50296
Conc: 0.54 ug/ml

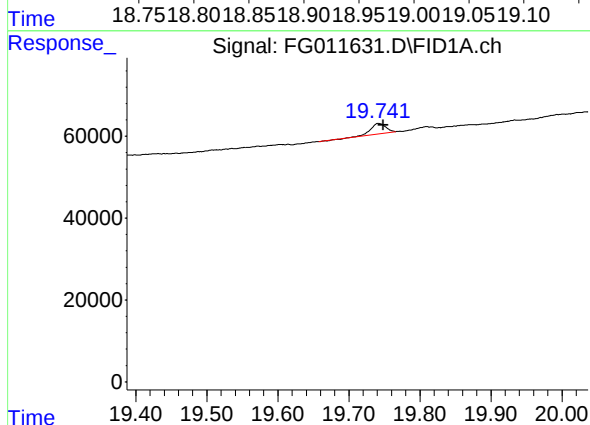

#15 N-TETRATRIACONTANE

R.T.: 19.742 min
Delta R.T.: -0.007 min
Response: 35620
Conc: 0.42 ug/ml