

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032023\
Data File : FG011624.D
Signal(s) : FID1A.ch
Acq On : 20 Mar 2023 12:34
Operator : YP\AJ
Sample : 01998-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 21 04:16:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.059	4032367	40.062 ug/ml
Target Compounds			


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032023\
Data File : FG011624.D
Signal(s) : FID1A.ch
Acq On : 20 Mar 2023 12:34
Operator : YP\AJ
Sample : 01998-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 21 04:16:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

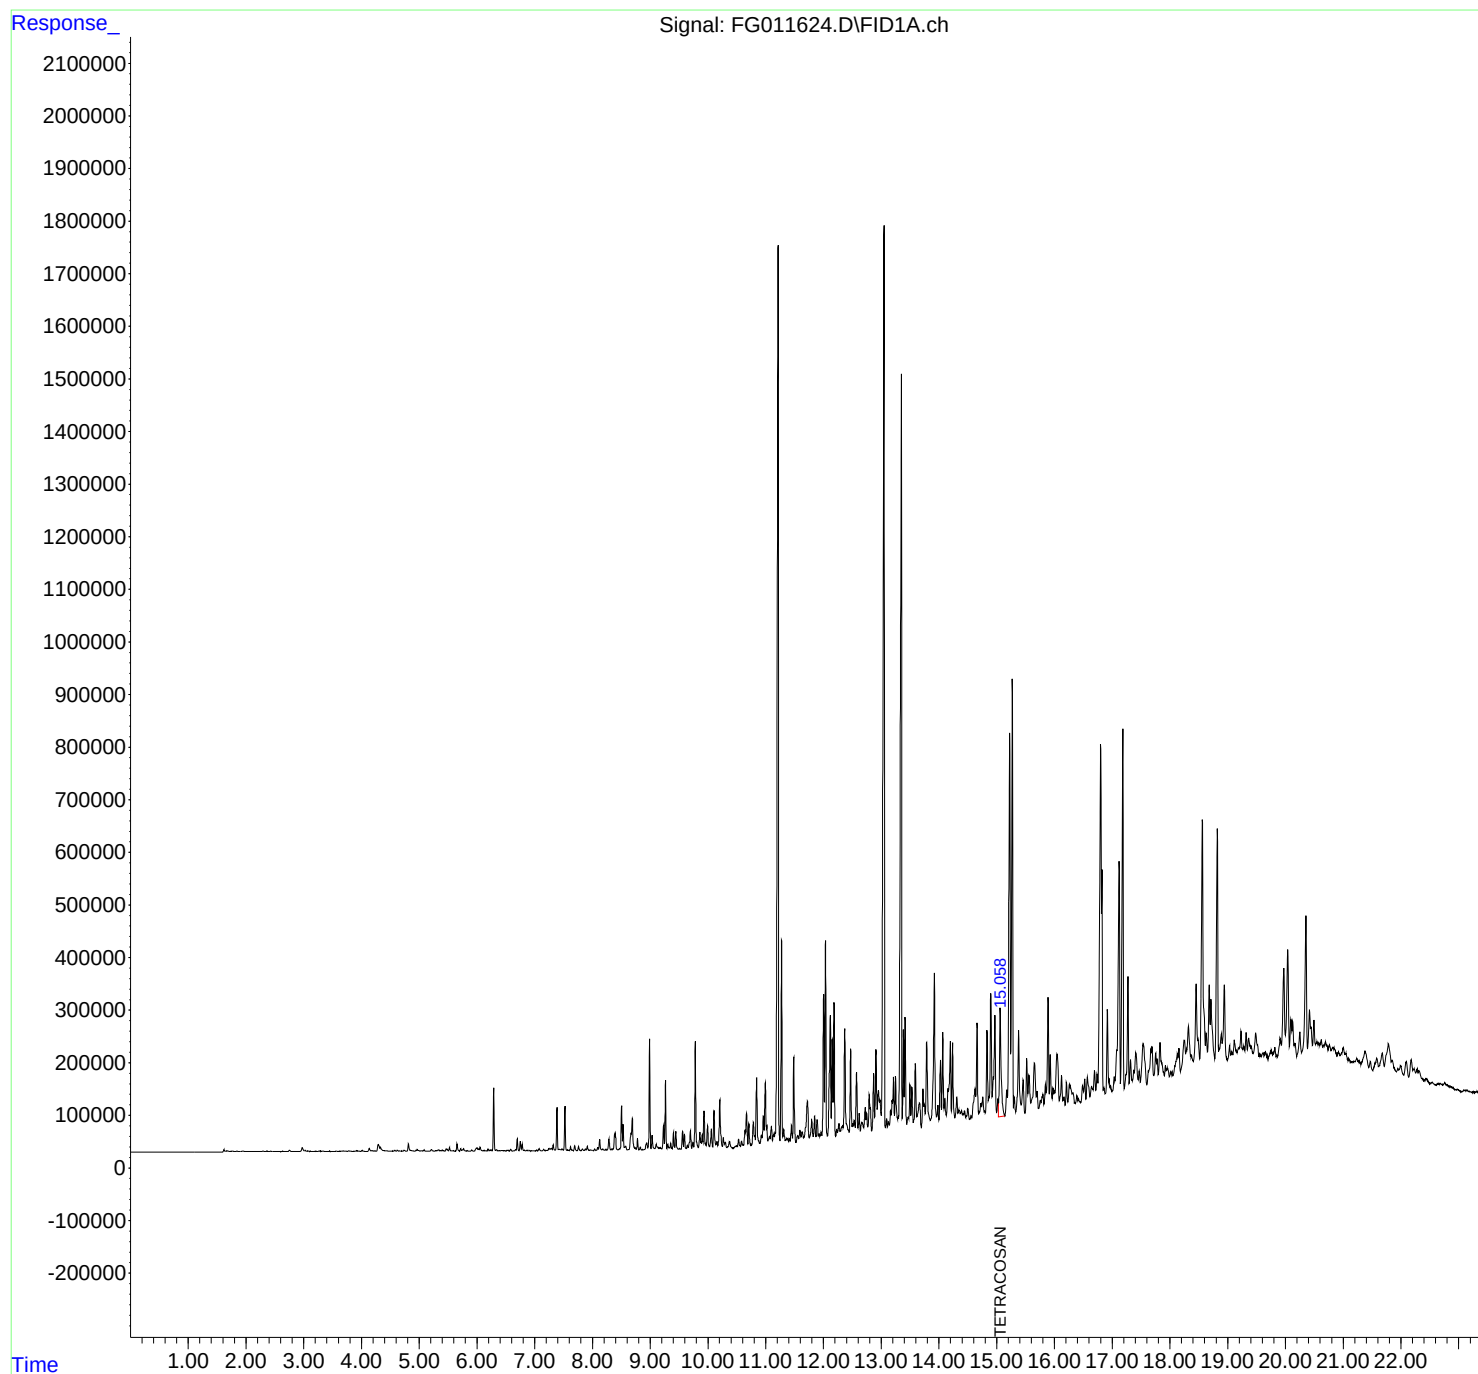

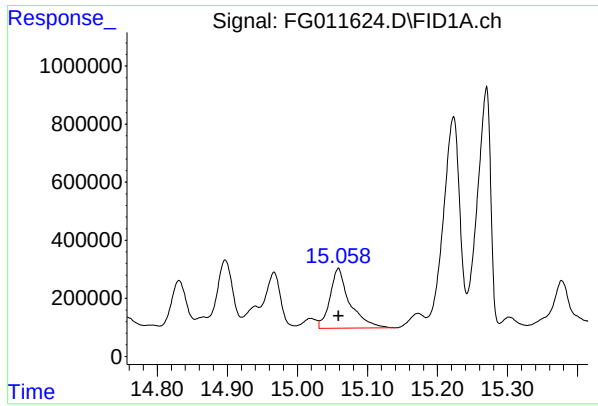

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.059 min
Delta R.T.: 0.000 min
Response: 4032367
Conc: 40.06 ug/ml