

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032119\
Data File : FG004301.D
Signal(s) : FID1A.ch
Acq On : 21 Mar 2019 11:50
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 22 01:27:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.183	2843310	20.973 ug/ml
12)	N-OCTACOSANE	16.605	2839454	20.740 ug/ml
13)	N-TRIACONTANE	17.492	207748	1.556 ug/ml
14)	N-DOTRIACONTANE	18.326	217641	1.720 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032119\
Data File : FG004301.D
Signal(s) : FID1A.ch
Acq On : 21 Mar 2019 11:50
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 22 01:27:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

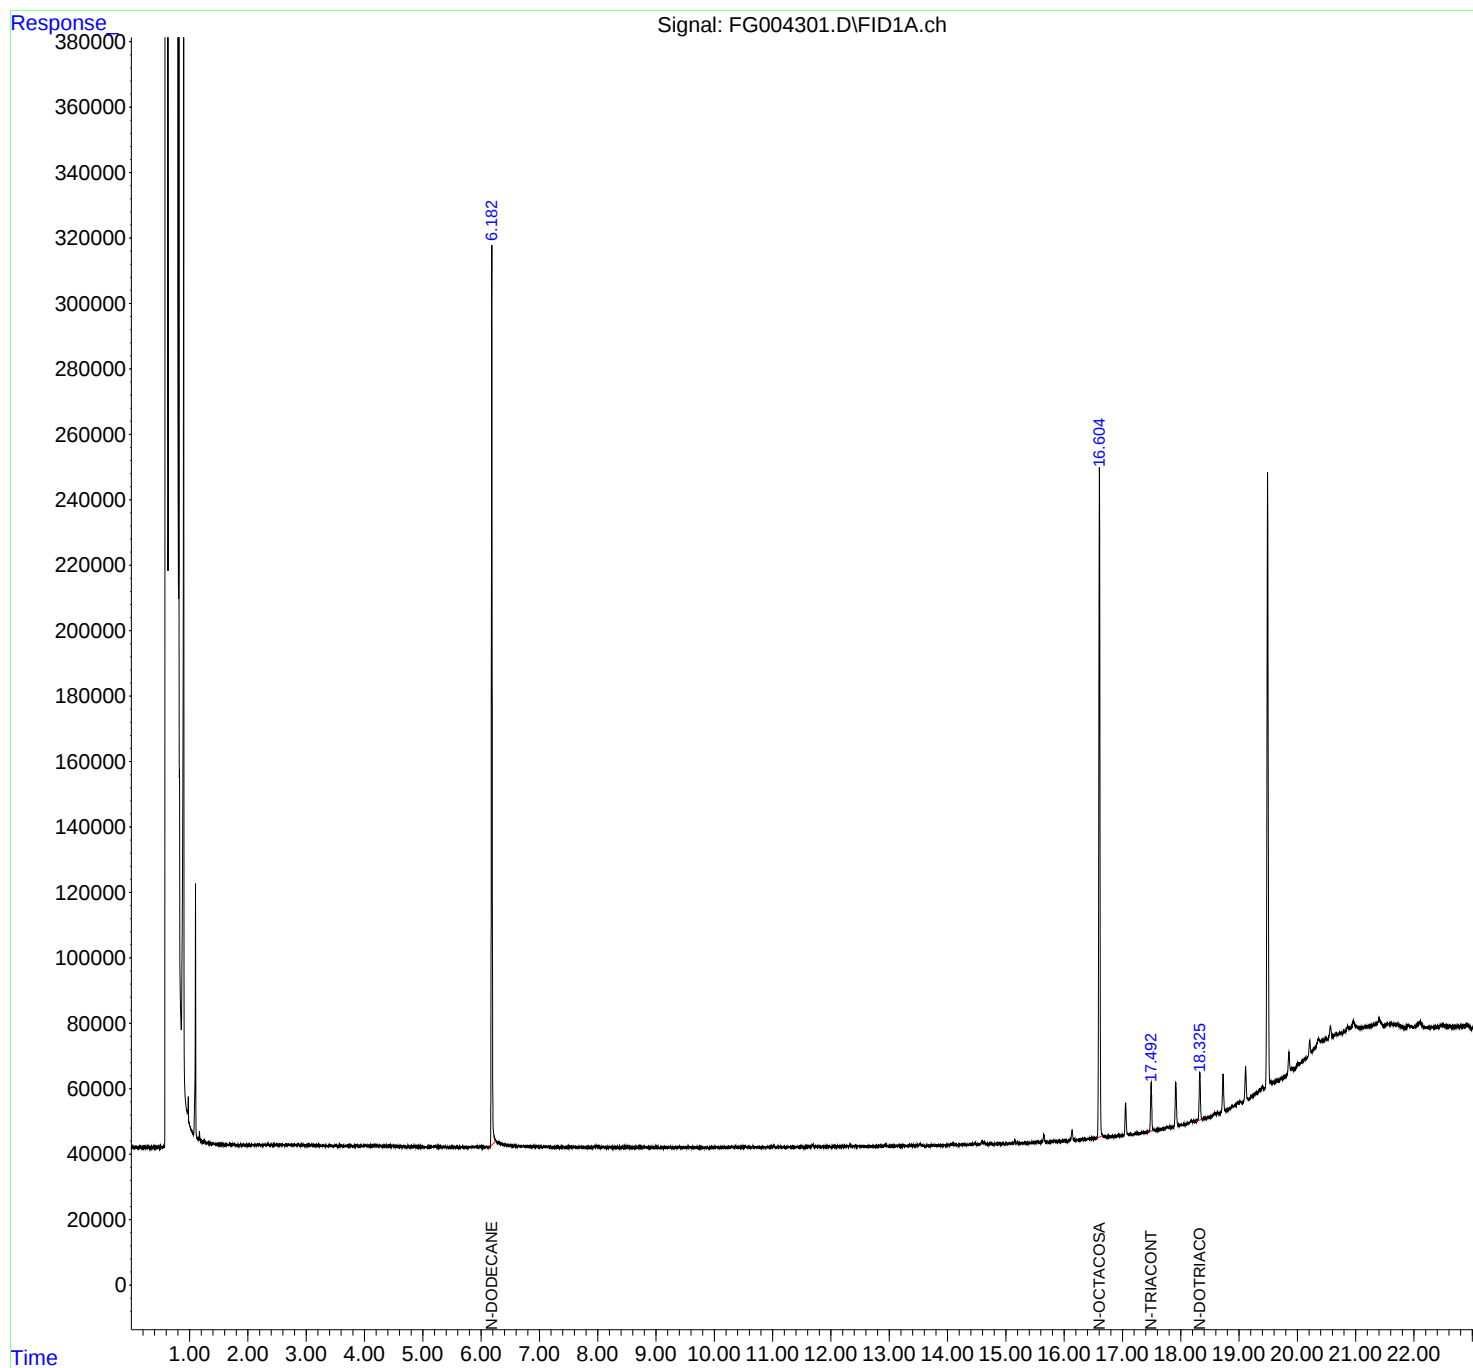


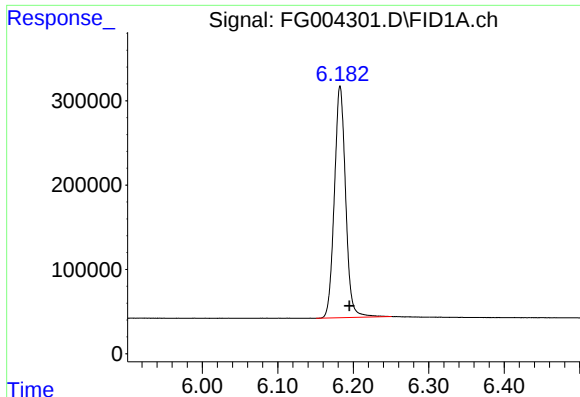

#3 N-DODECANE


R.T.: 6.183 min
Delta R.T.: -0.012 min
Response: 2843310
Conc: 20.97 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

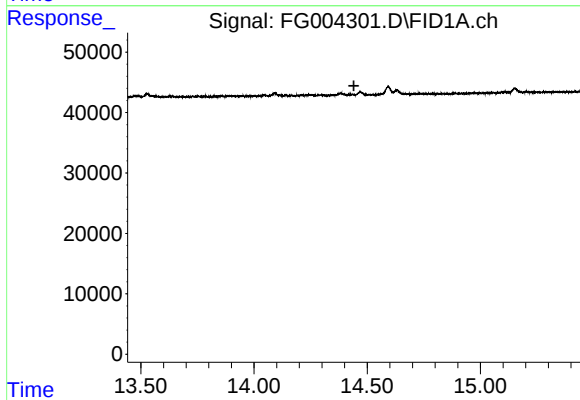


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.441 min
Response: 0
Conc: N.D.

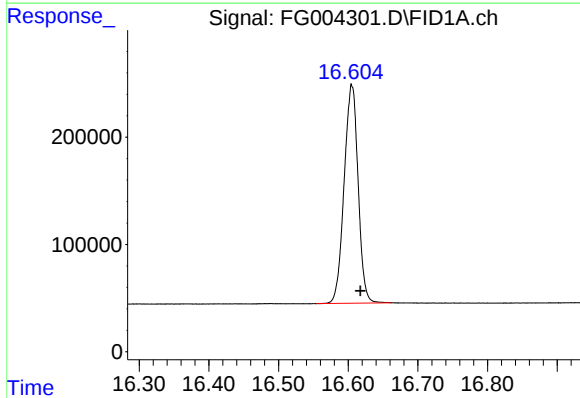


#12 N-OCTACOSANE

R.T.: 16.605 min
Delta R.T.: -0.012 min
Response: 2839454
Conc: 20.74 ug/ml

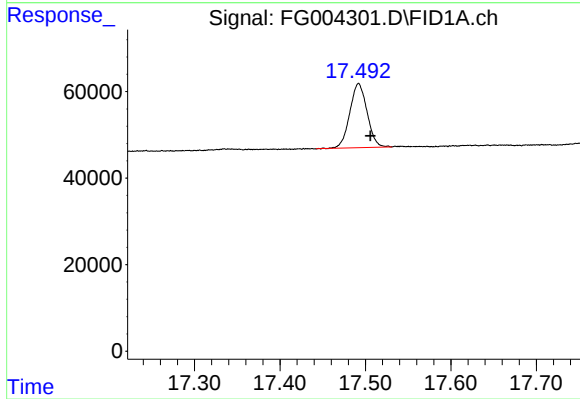

#13 N-TRIACONTANE

R.T.: 17.492 min
Delta R.T.: -0.014 min
Response: 207748
Conc: 1.56 ug/ml

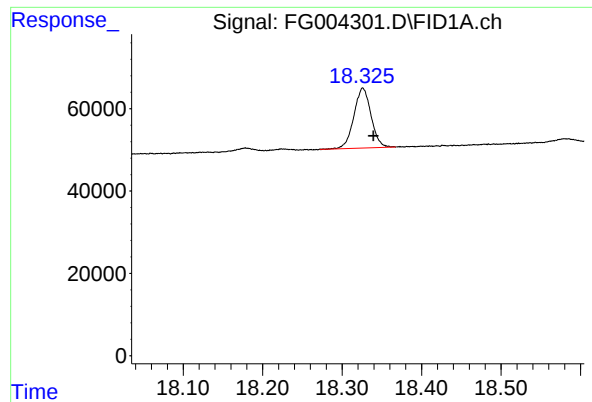

#14 N-DOTRIACONTANE

R.T.: 18.326 min
Delta R.T.: -0.013 min
Response: 217641
Conc: 1.72 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER