

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032119\
 Data File : FG004316.D
 Signal(s) : FID1A.ch
 Acq On : 21 Mar 2019 19:58
 Operator : AJ\SJ
 Sample : K2036-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 SIMW-04-20190319

Integration File: autoint1.e
 Quant Time: Mar 22 01:33:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
 Quant Title :
 QLast Update : Tue Mar 05 03:05:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.428	2087580	16.605 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032119\
Data File : FG004316.D
Signal(s) : FID1A.ch
Acq On : 21 Mar 2019 19:58
Operator : AJ\SJ
Sample : K2036-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SIMW-04-20190319

Integration File: autoint1.e
Quant Time: Mar 22 01:33:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

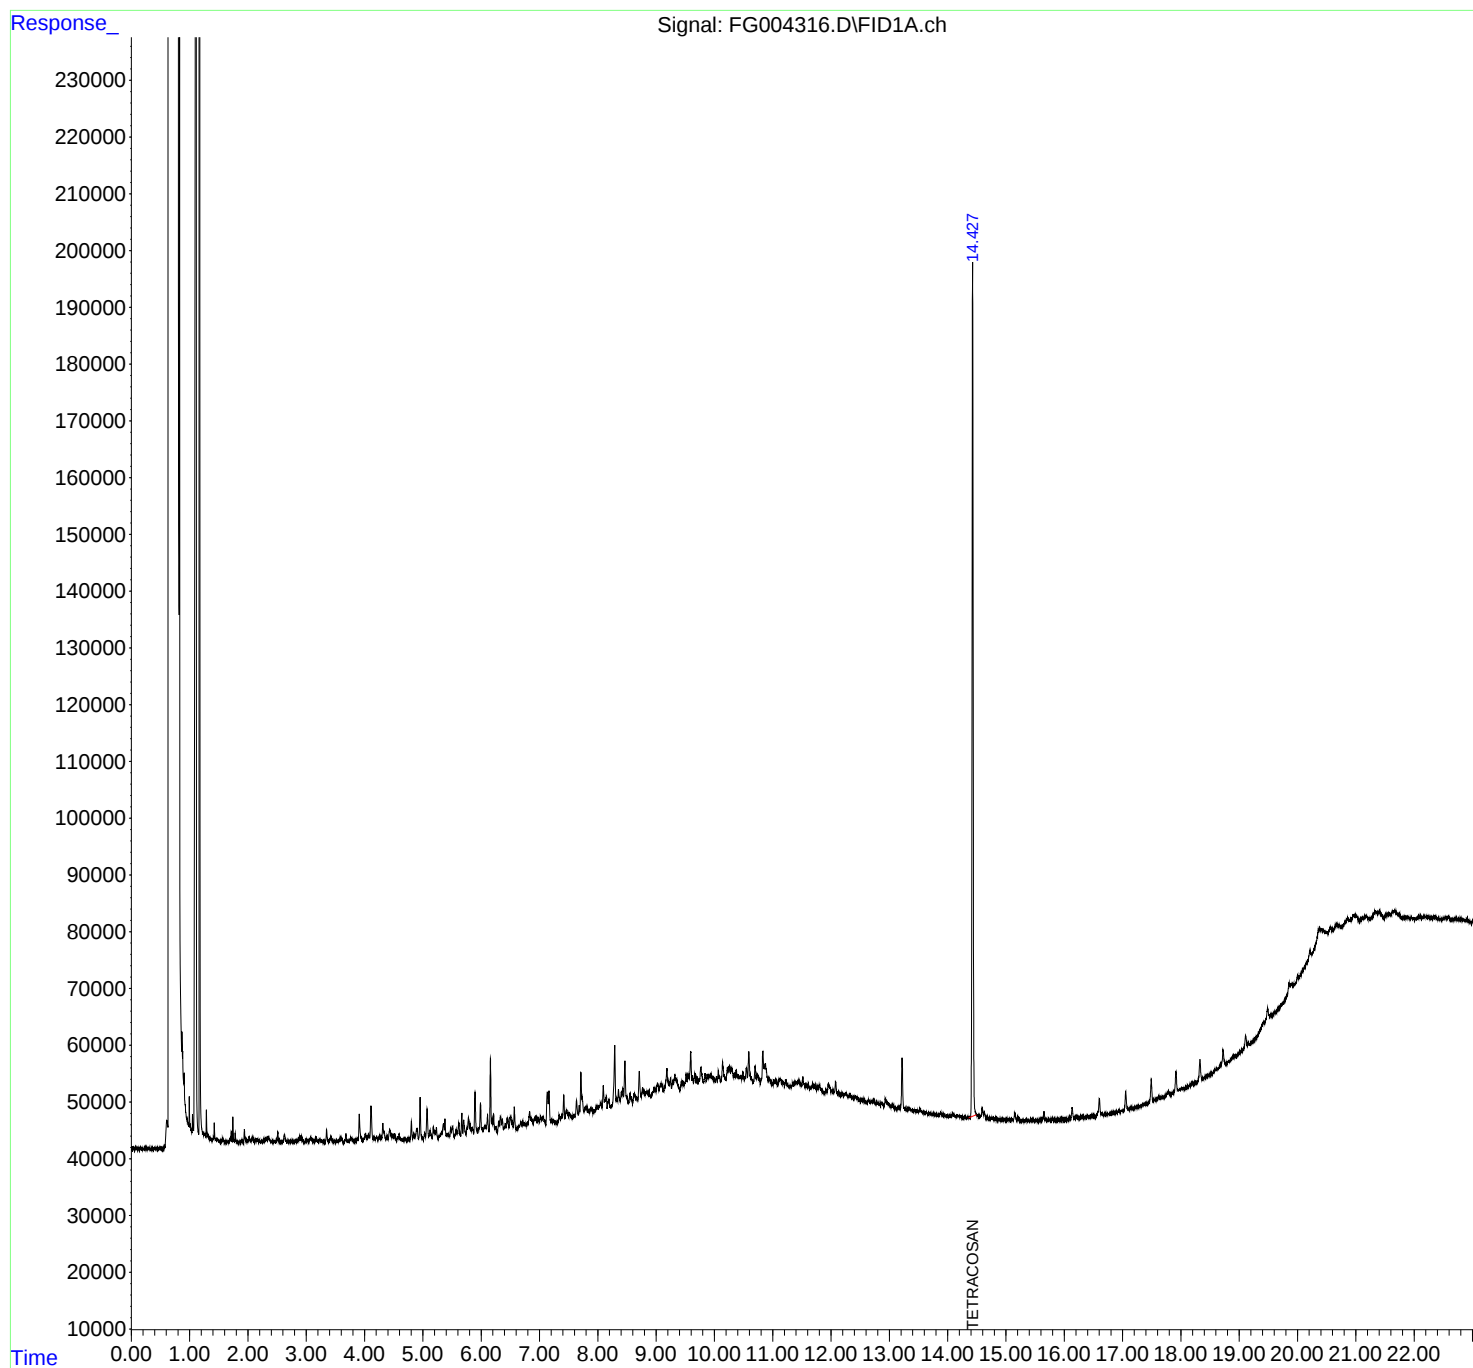

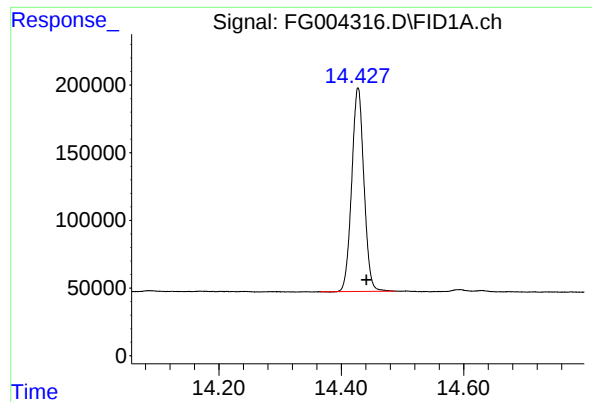

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.428 min
Delta R.T.: -0.014 min
Response: 2087580
Conc: 16.61 ug/ml

Instrument :
FID_G
ClientSampleId :
SIMW-04-20190319