

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032119\
 Data File : FG004324.D
 Signal(s) : FID1A.ch
 Acq On : 22 Mar 2019 00:01
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Mar 22 01:34:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
 Quant Title :
 QLast Update : Tue Mar 05 03:05:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.426	1891501	15.045 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.492	195150	1.461 ug/ml
14) N-DOTRIACONTANE	18.330	352285	2.784 ug/ml
16) N-HEXATRIACONTANE	19.893	329580	2.977 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032119\
Data File : FG004324.D
Signal(s) : FID1A.ch
Acq On : 22 Mar 2019 00:01
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 22 01:34:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

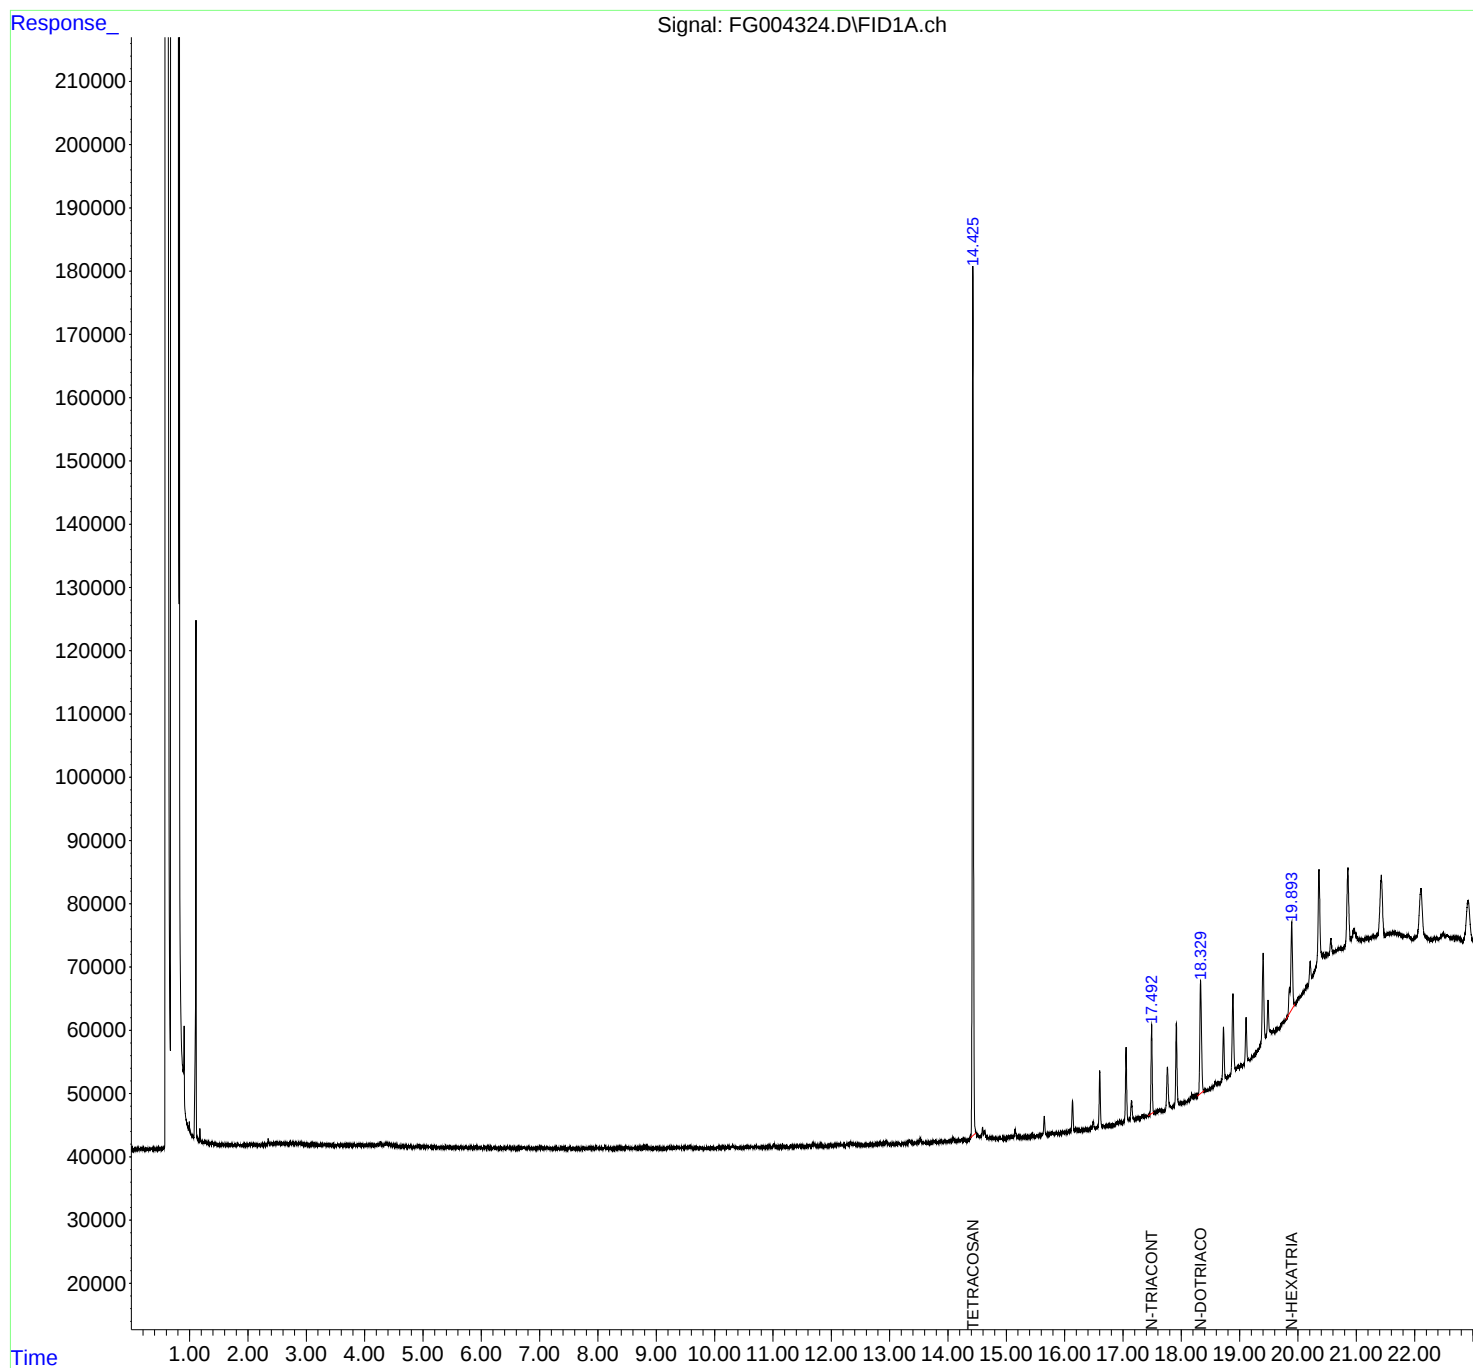


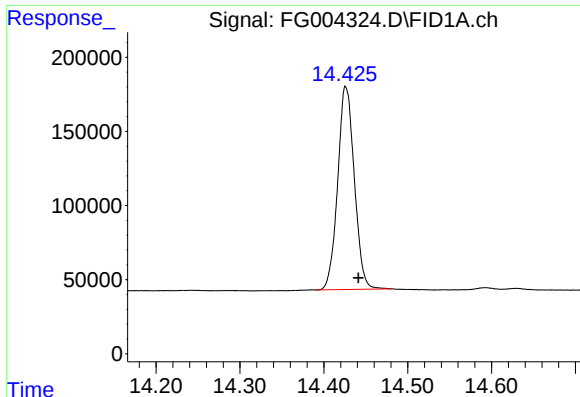

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.426 min
Delta R.T.: -0.015 min
Response: 1891501
Conc: 15.05 ug/ml

Instrument :
FID_G
ClientSampleId :
I.BLK

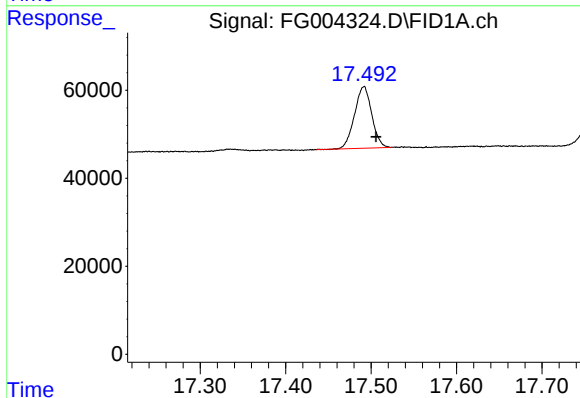


#13 N-TRIACONTANE

R.T.: 17.492 min
Delta R.T.: -0.014 min
Response: 195150
Conc: 1.46 ug/ml

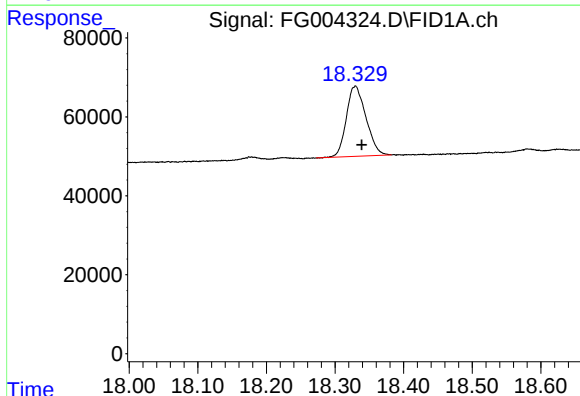

#14 N-DOTRIACONTANE

R.T.: 18.330 min
Delta R.T.: -0.009 min
Response: 352285
Conc: 2.78 ug/ml

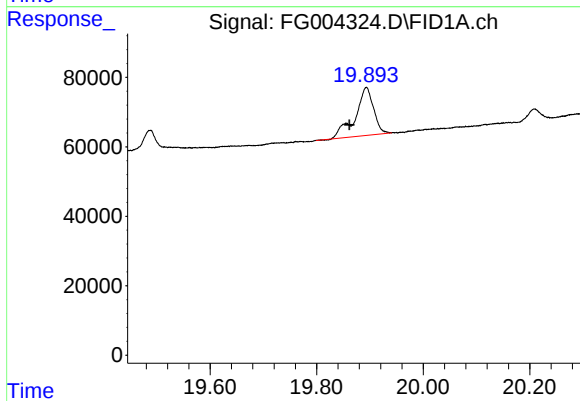

#16 N-HEXATRIACONTANE

R.T.: 19.893 min
Delta R.T.: 0.031 min
Response: 329580
Conc: 2.98 ug/ml