

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032119\
Data File : FG004315.D
Signal(s) : FID1A.ch
Acq On : 21 Mar 2019 19:28
Operator : AJ\SJ
Sample : K2036-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SIMW-02-20190319-A

Integration File: Sample.e
Quant Time: Mar 22 01:33:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.428	1807018	14.373 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032119\
Data File : FG004315.D
Signal(s) : FID1A.ch
Acq On : 21 Mar 2019 19:28
Operator : AJ\SJ
Sample : K2036-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SIMW-02-20190319-A

Integration File: Sample.e
Quant Time: Mar 22 01:33:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

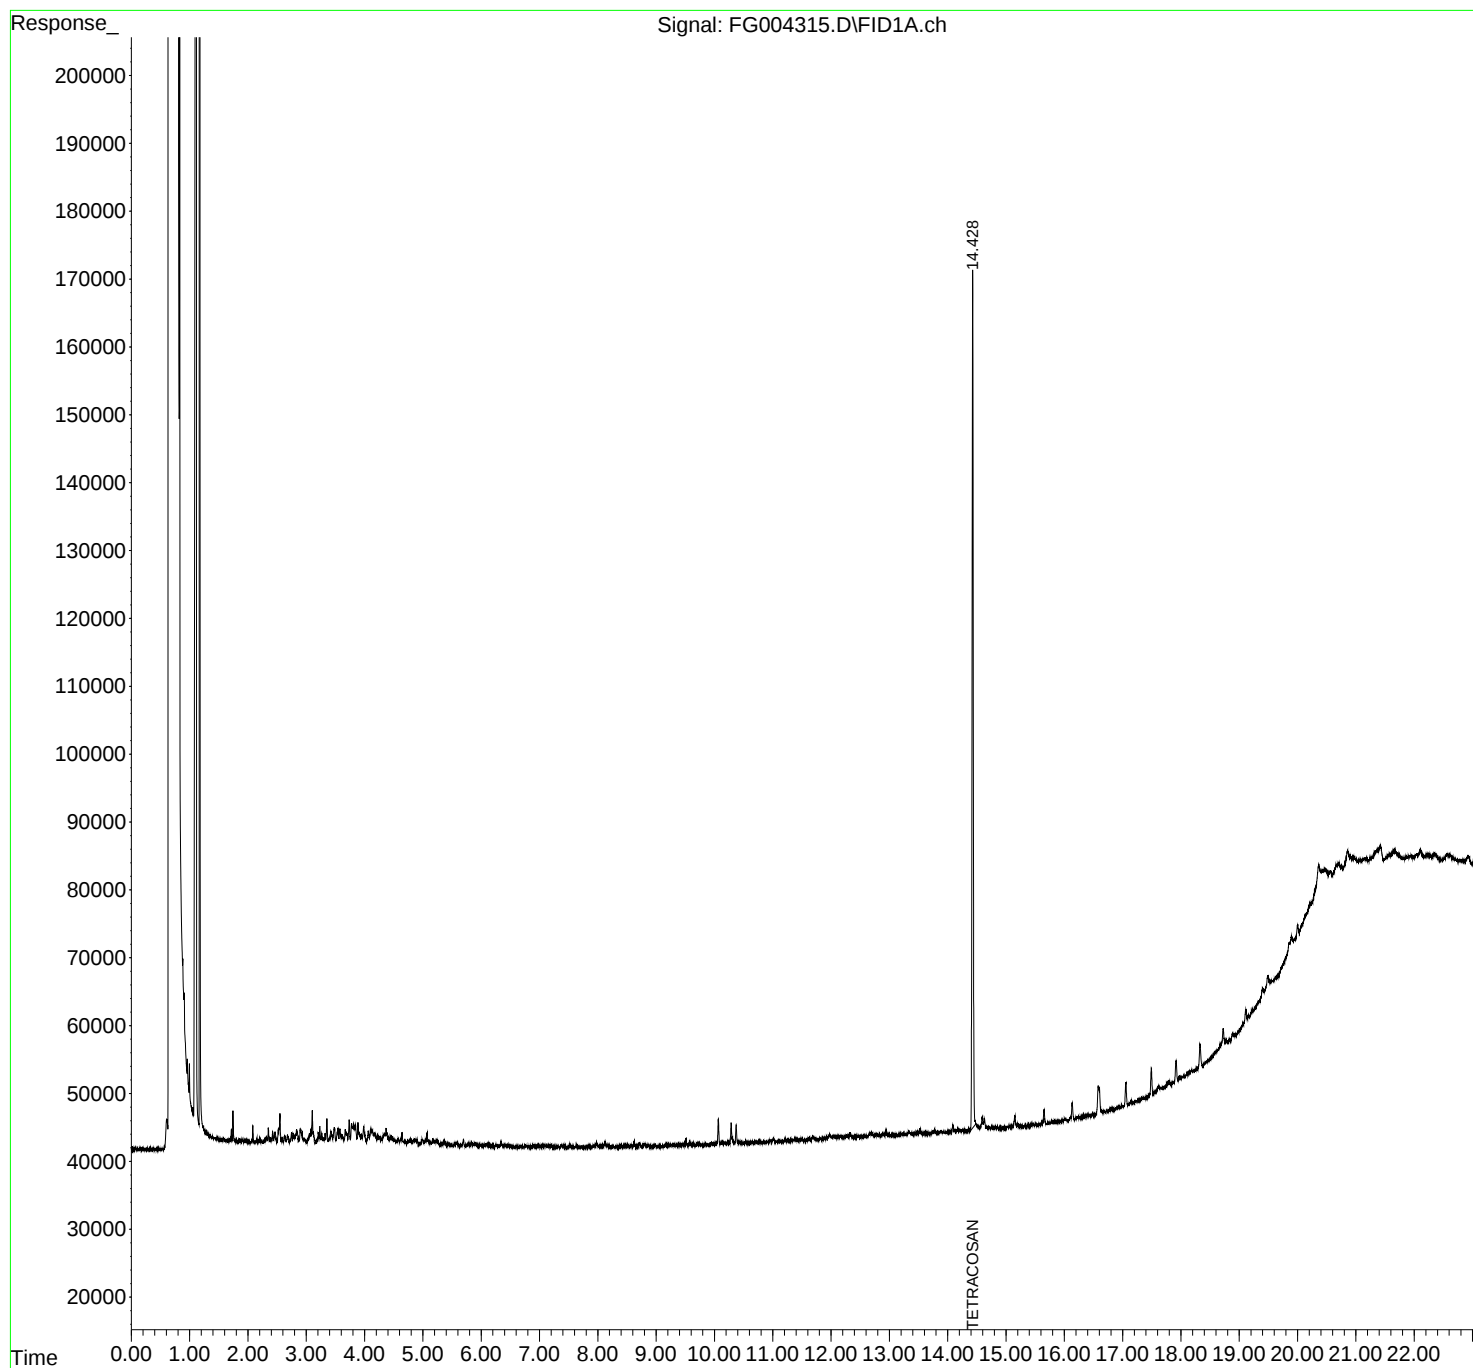

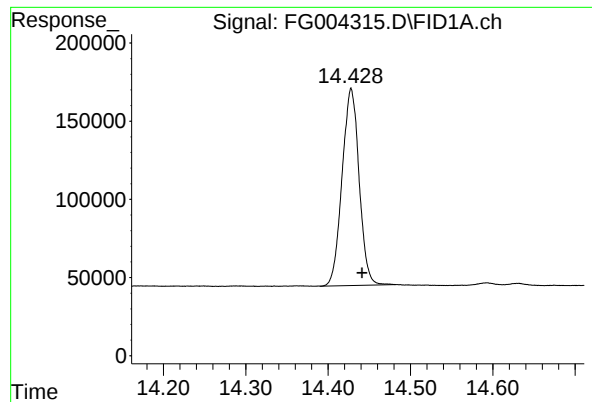

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.428 min
Delta R.T.: -0.013 min
Response: 1807018
Conc: 14.37 ug/ml

Instrument :
FID_G
ClientSampleId :
SIMW-02-20190319-A