

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032125AR\
Data File : FG015531.D
Signal(s) : FID1A.ch
Acq On : 21 Mar 2025 07:56
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Mar 21 22:52:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aromatic EPH 031725.M
Quant Title : GC Extractables
QLast Update : Tue Mar 18 05:13:04 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

14) T	Benzo[a]anthracene (C...	15.199	1244266	9.174 ug/ml
15) T	Chrysene (C27.41)	15.199	1244266	8.888 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032125AR\
Data File : FG015531.D
Signal(s) : FID1A.ch
Acq On : 21 Mar 2025 07:56
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Mar 21 22:52:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aromatic EPH 031725.M
Quant Title : GC Extractables
QLast Update : Tue Mar 18 05:13:04 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

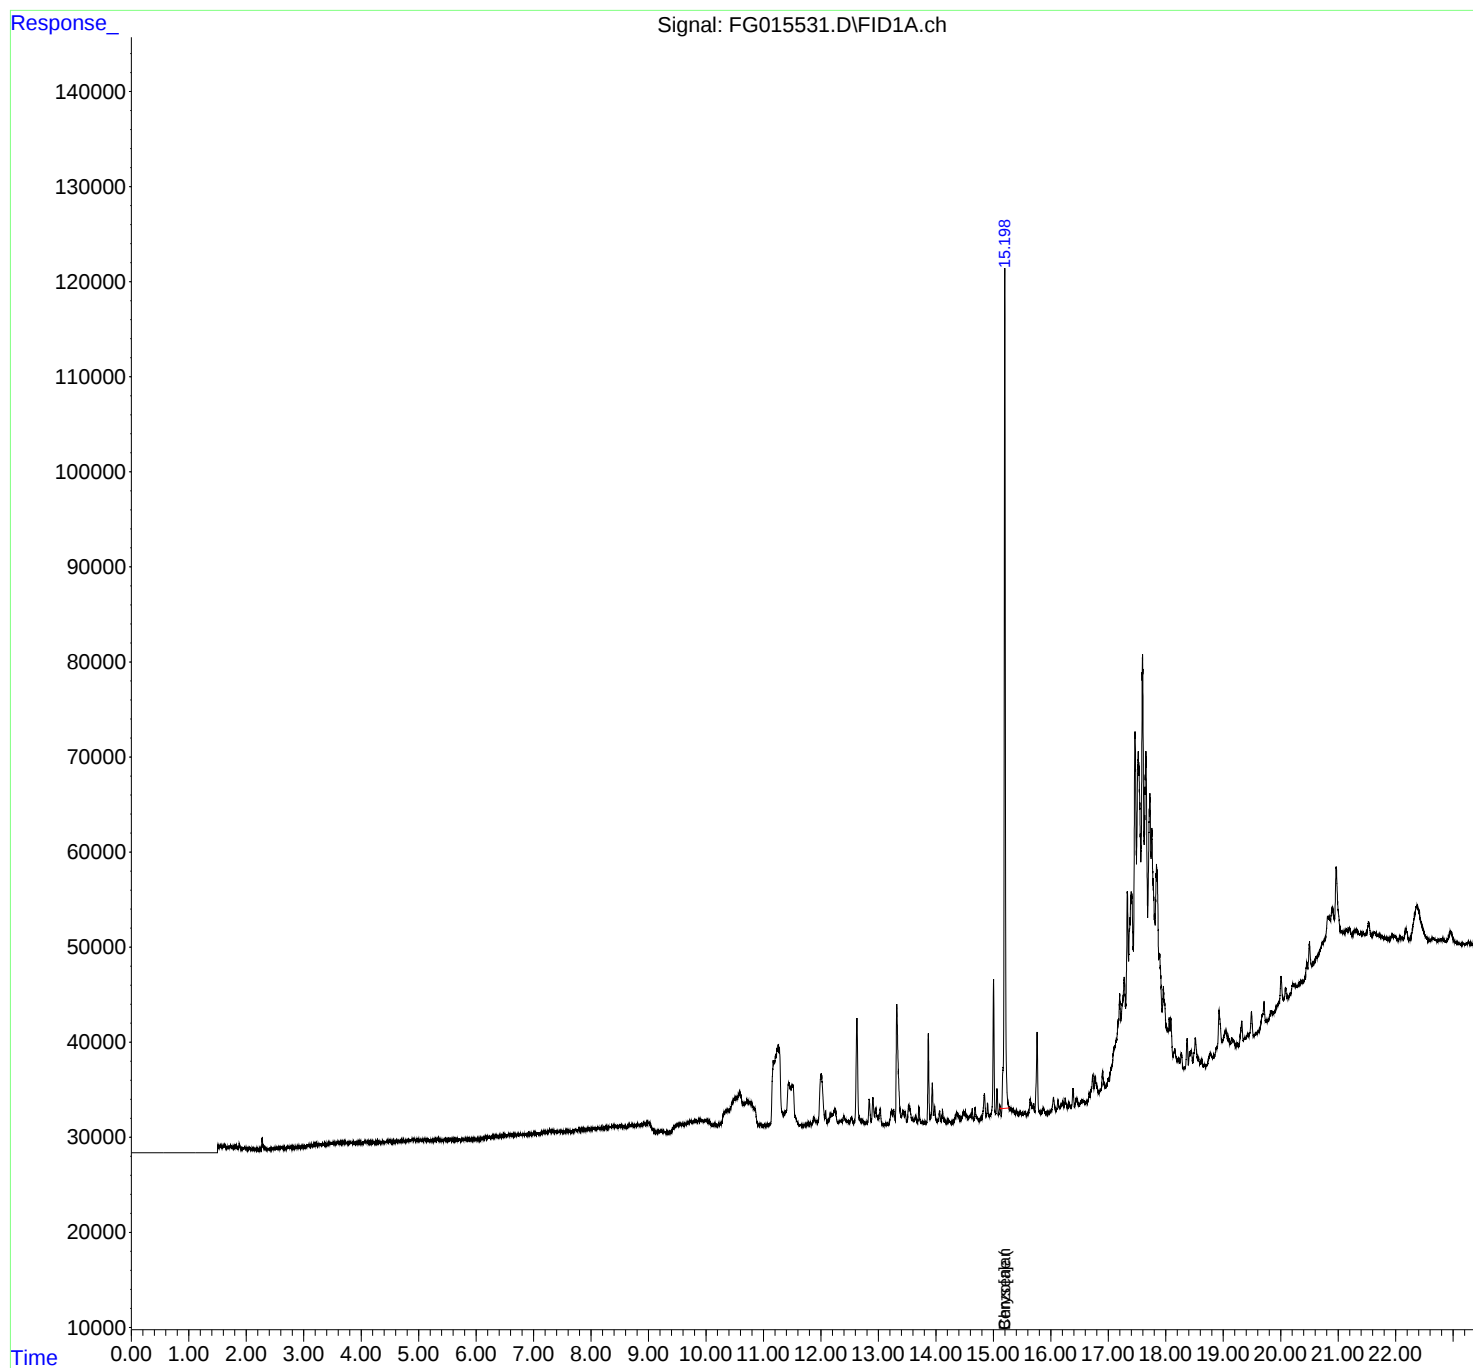


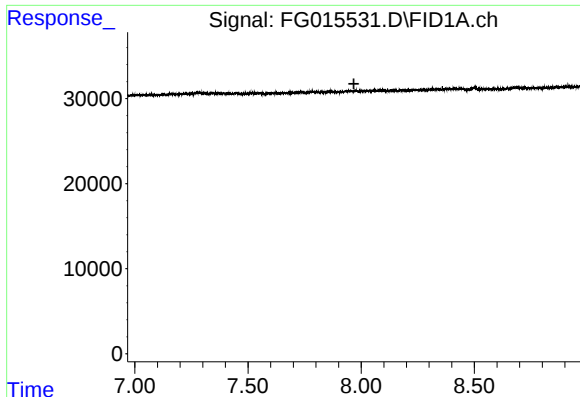

#4 2-Bromonaphthalene (SURRE)


R.T.: 0.000 min
Exp R.T. : 7.968 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :
MECL2

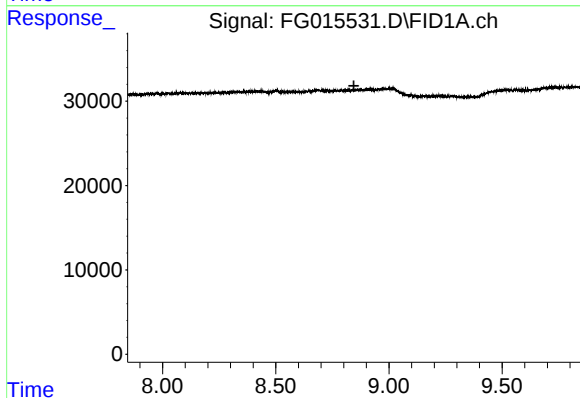


#6 2-Fluorobiphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 8.845 min
Response: 0
Conc: N.D.

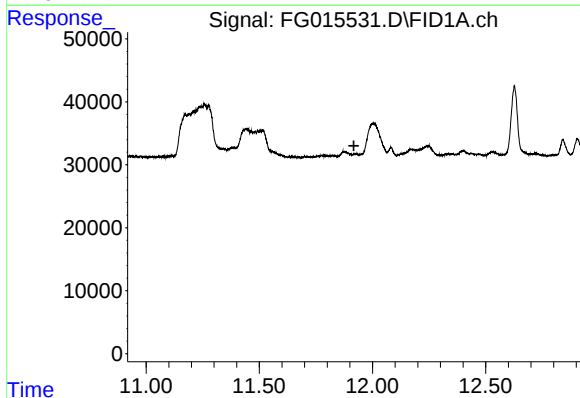


#11 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 11.918 min
Response: 0
Conc: N.D.

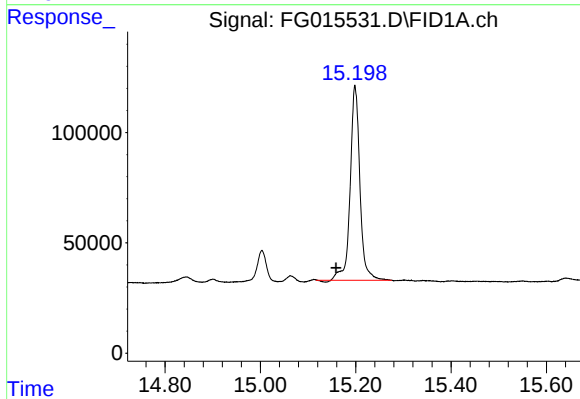

#14 Benzo[a]anthracene (C26.37)

R.T.: 15.199 min
Delta R.T.: 0.040 min
Response: 1244266
Conc: 9.17 ug/ml

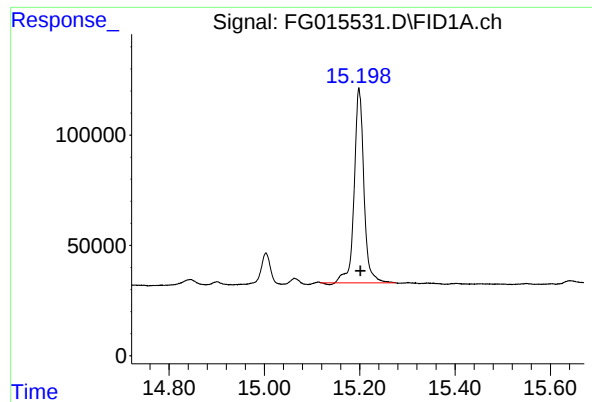

#15 Chrysene (C27.41)

R.T.: 15.199 min
Delta R.T.: -0.002 min
Response: 1244266
Conc: 8.89 ug/ml

Instrument :
FID_G
ClientSampleId :
MECL2