

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032323\
 Data File : FG011653.D
 Signal(s) : FID1A.ch
 Acq On : 23 Mar 2023 23:37
 Operator : YP\AJ
 Sample : 02045-05 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 24 02:12:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
 Quant Title :
 QLast Update : Wed Mar 15 18:43:49 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.046	165766	1.647 ug/ml
Target Compounds			
7) N-EICOSANE	13.011f	319288	2.657 ug/ml
10) N-TETRACOSANE	15.234	188682	1.670 ug/ml
12) N-OCTACOSANE	17.238	58509	0.564 ug/ml
14) N-DOTRIACONTANE	18.901f	53941	0.582 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032323\
Data File : FG011653.D
Signal(s) : FID1A.ch
Acq On : 23 Mar 2023 23:37
Operator : YP\AJ
Sample : 02045-05 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 24 02:12:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

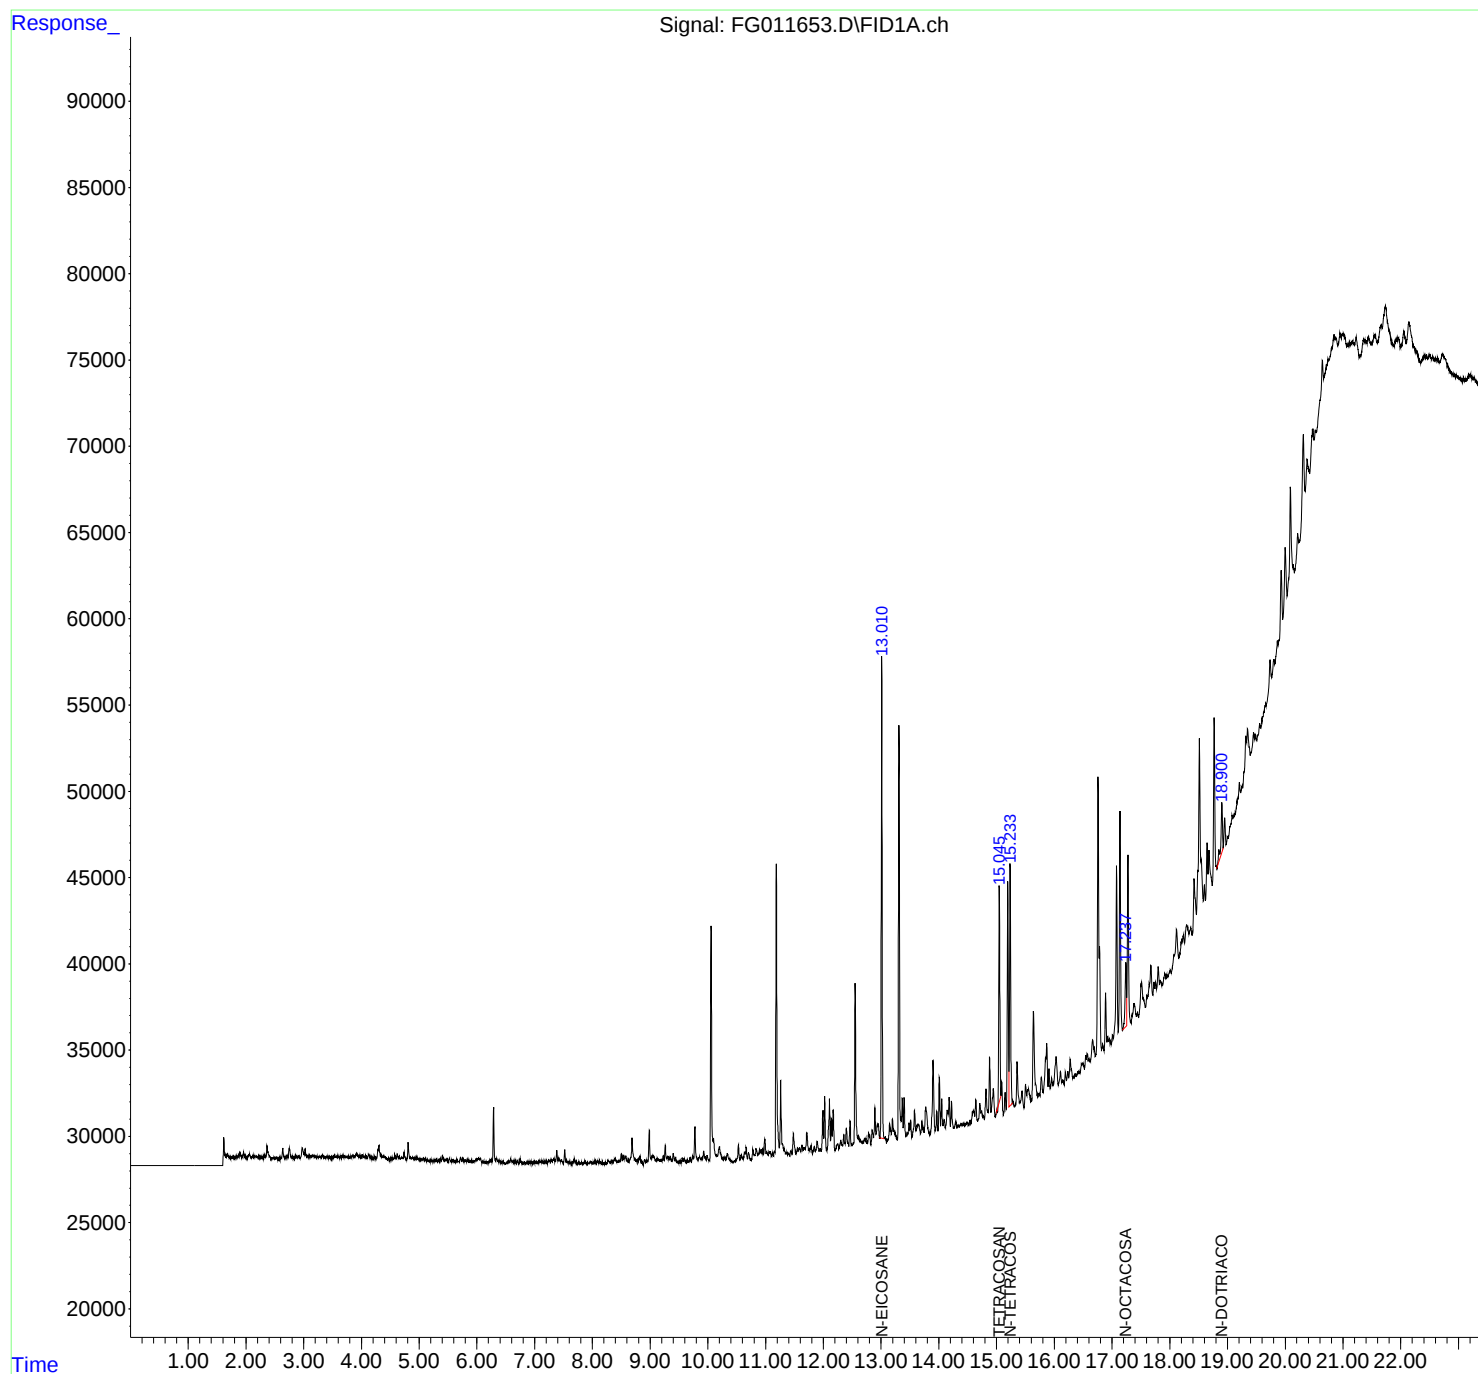


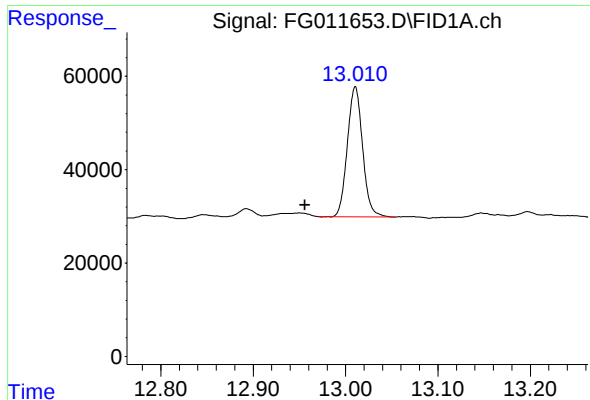

#7 N-EICOSANE


R.T.: 13.011 min
Delta R.T.: 0.054 min
Response: 319288
Conc: 2.66 ug/ml

Instrument :
FID_G
ClientSampleId :

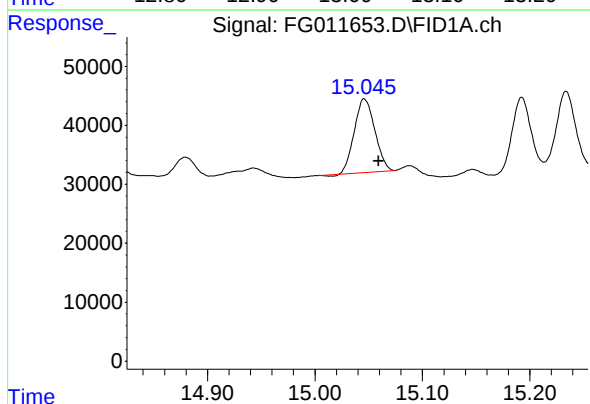


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.046 min
Delta R.T.: -0.013 min
Response: 165766
Conc: 1.65 ug/ml

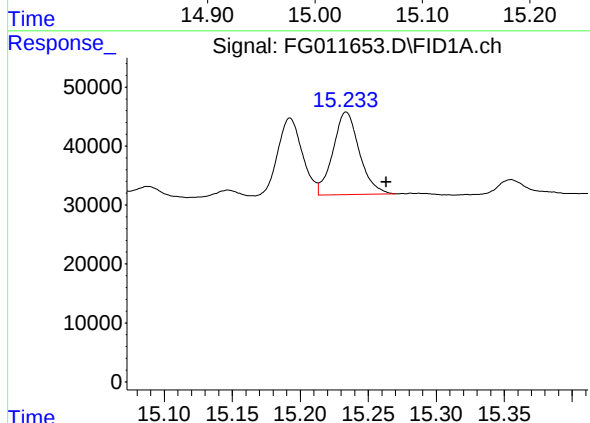


#10 N-TETRACOSANE

R.T.: 15.234 min
Delta R.T.: -0.030 min
Response: 188682
Conc: 1.67 ug/ml

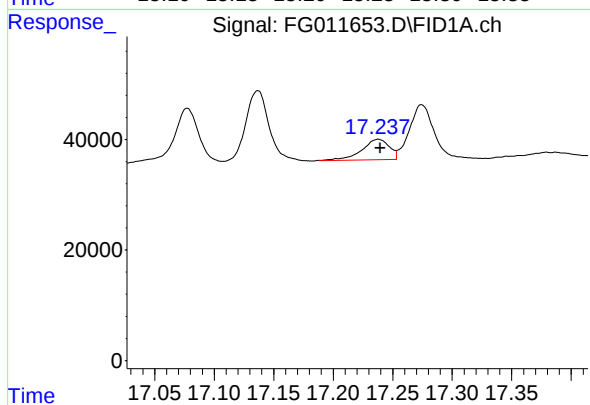

#12 N-OCTACOSANE

R.T.: 17.238 min
Delta R.T.: -0.002 min
Response: 58509
Conc: 0.56 ug/ml

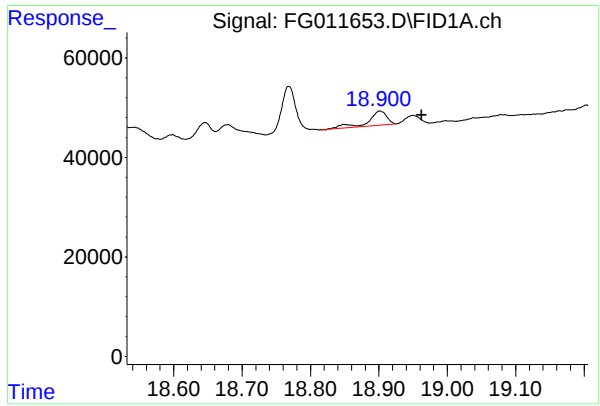

#14 N-DOTRIACONTANE

R.T.: 18.901 min
Delta R.T.: -0.061 min
Response: 53941
Conc: 0.58 ug/ml

Instrument :

FID_G

ClientSampleId :