

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032323\
 Data File : FG011636.D
 Signal(s) : FID1A.ch
 Acq On : 23 Mar 2023 11:05
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Mar 24 02:10:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
 Quant Title :
 QLast Update : Wed Mar 15 18:43:49 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.745	1944083	15.932 ug/ml
12) N-OCTACOSANE	17.223	1931765	18.630 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032323\
Data File : FG011636.D
Signal(s) : FID1A.ch
Acq On : 23 Mar 2023 11:05
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 24 02:10:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

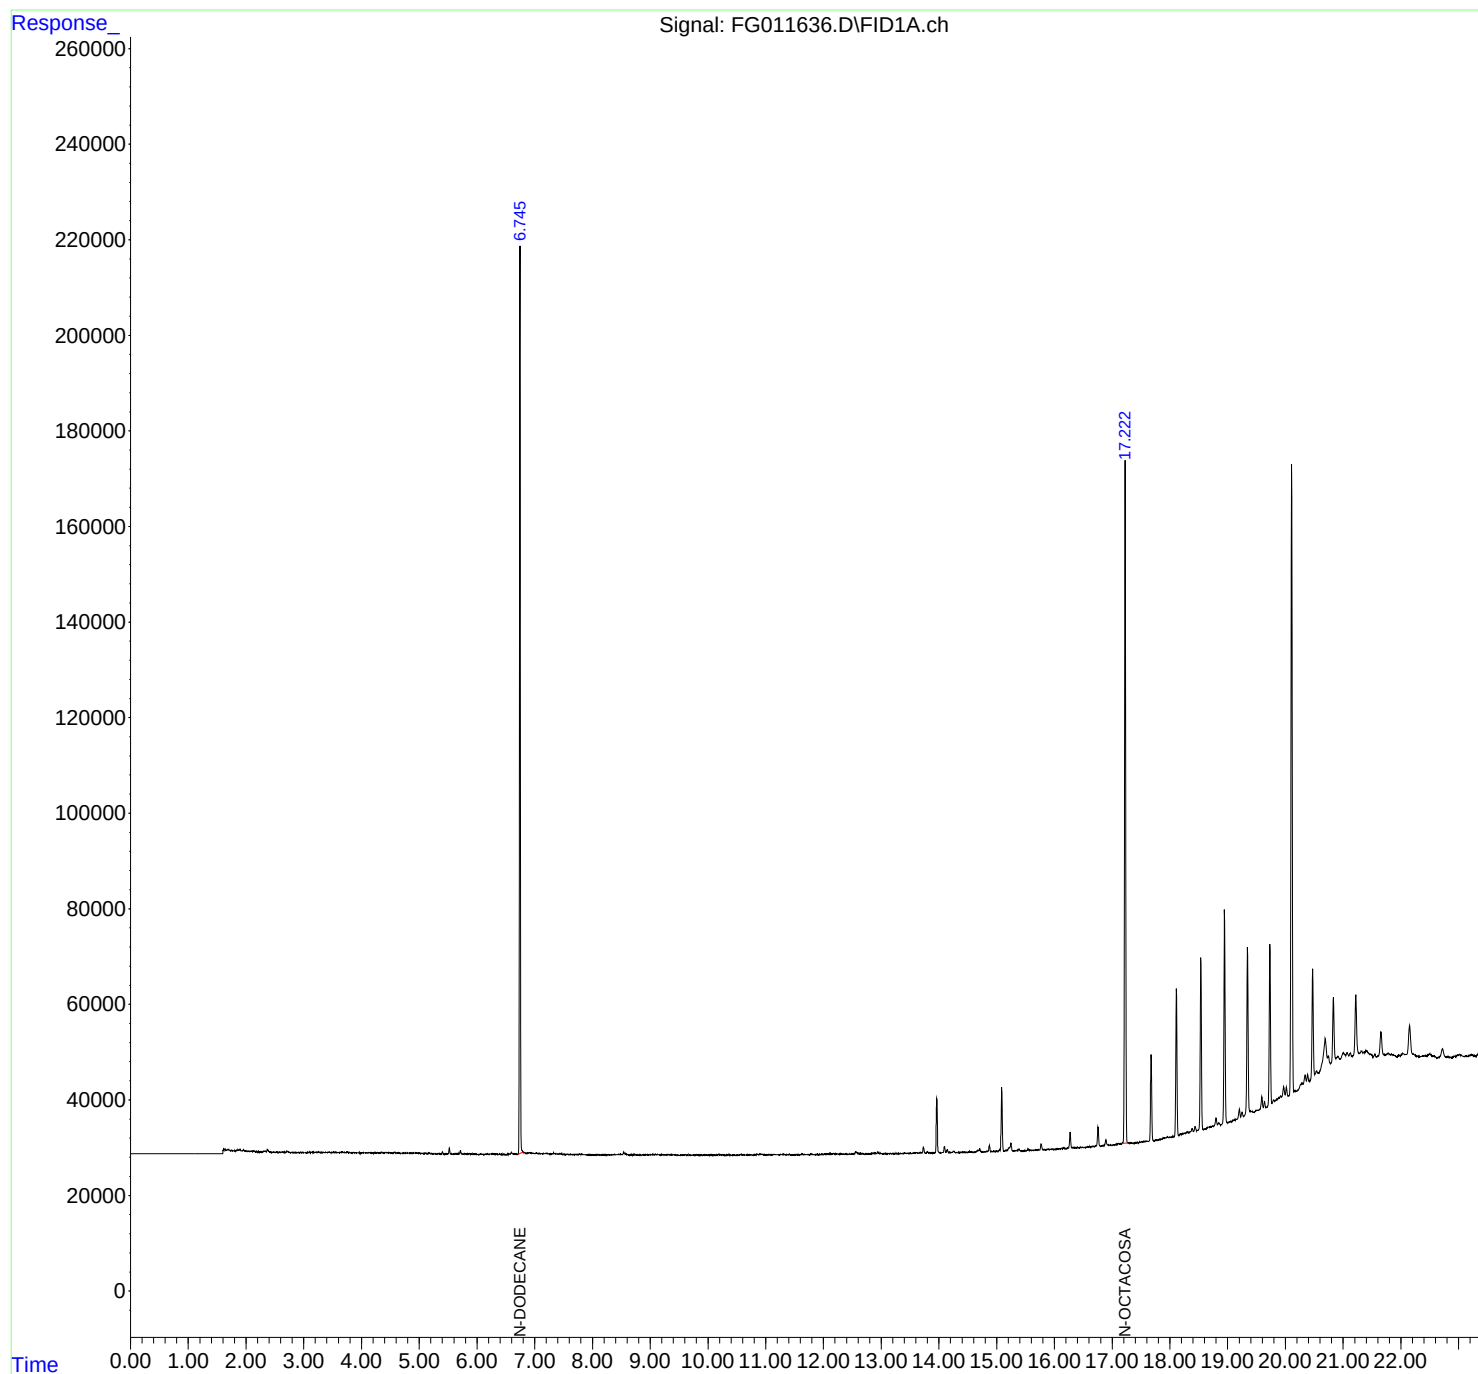


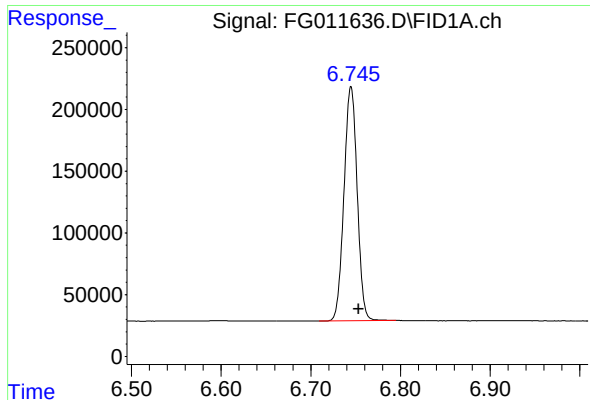

#3 N-DODECANE


R.T.: 6.745 min
Delta R.T.: -0.009 min
Response: 1944083
Conc: 15.93 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

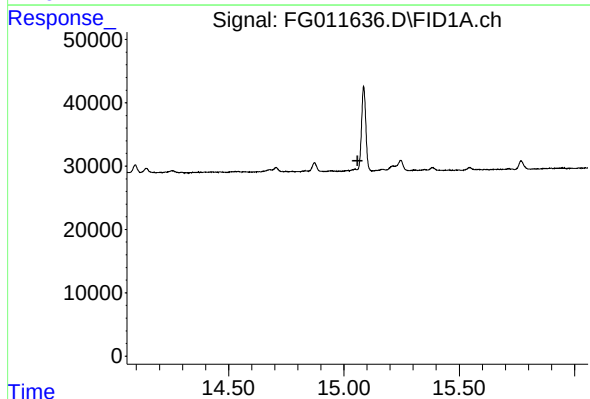

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.059 min
Response: 0
Conc: N.D.

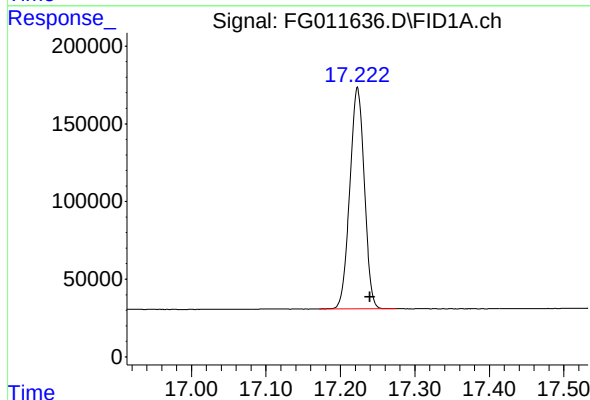

#12 N-OCTACOSANE

R.T.: 17.223 min
Delta R.T.: -0.017 min
Response: 1931765
Conc: 18.63 ug/ml