

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032323\
 Data File : FG011645.D
 Signal(s) : FID1A.ch
 Acq On : 23 Mar 2023 18:37
 Operator : YP\AJ
 Sample : 02045-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 WC1-20230322

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/24/2023
 Supervised By :Ankita Jodhani 03/24/2023

Integration File: autoint1.e
 Quant Time: Mar 24 02:11:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
 Quant Title :
 QLast Update : Wed Mar 15 18:43:49 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.055	1956823	19.441 ug/mlm

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032323\
Data File : FG011645.D
Signal(s) : FID1A.ch
Acq On : 23 Mar 2023 18:37
Operator : YP\AJ
Sample : 02045-06
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
WC1-20230322


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/24/2023
Supervised By :Ankita Jodhani 03/24/2023

Integration File: autoint1.e
Quant Time: Mar 24 02:11:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

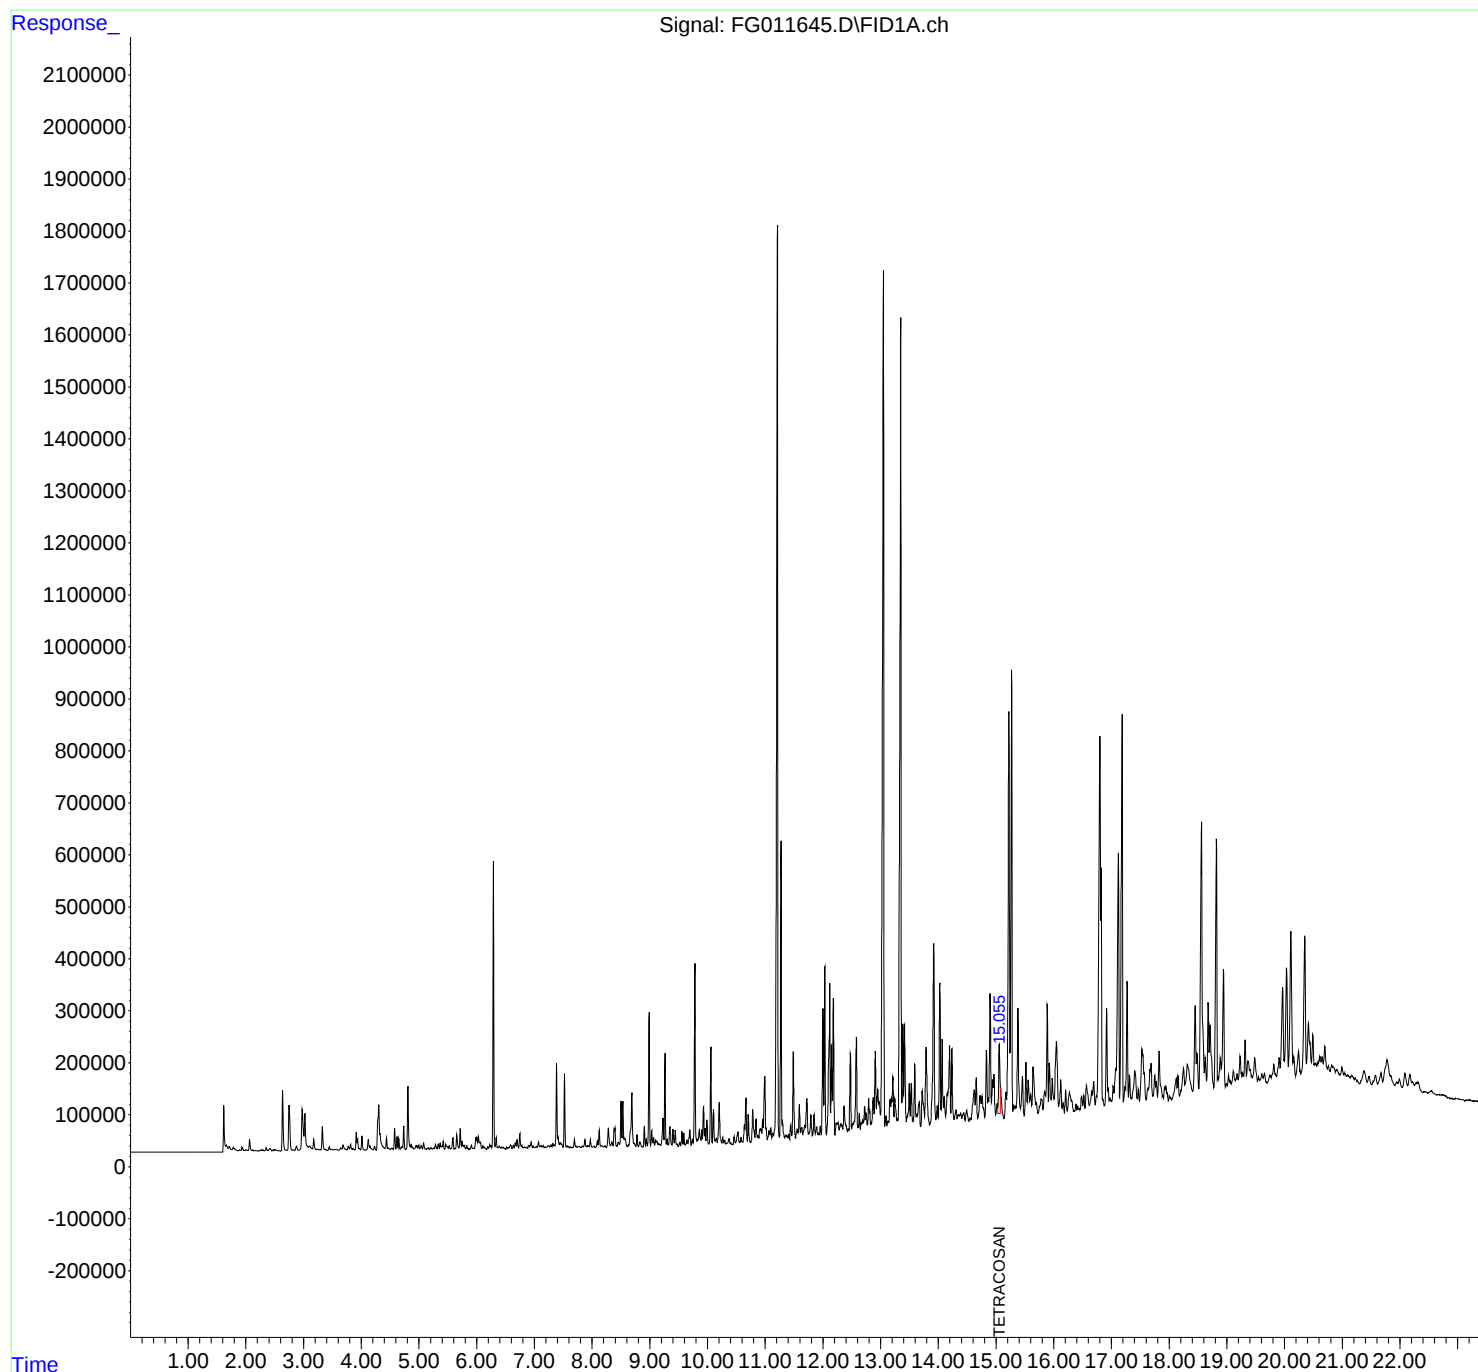

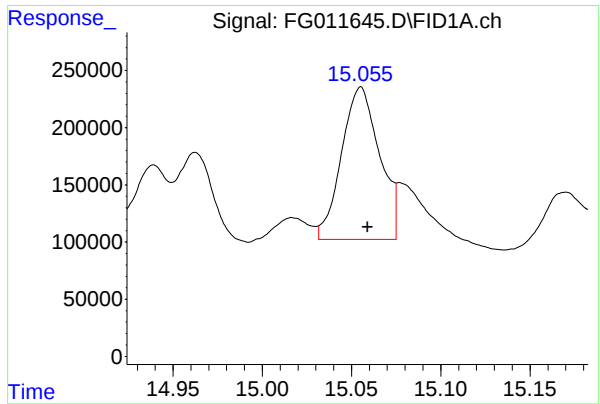

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.055 min
Delta R.T.: -0.004 min
Response: 1956823
Conc: 19.44 ug/ml

Instrument :

FID_G

ClientSampleId :

WC1-20230322

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 03/24/2023
Supervised By :Ankita Jodhani 03/24/2023