

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032323\
Data File : FG011647.D
Signal(s) : FID1A.ch
Acq On : 23 Mar 2023 19:37
Operator : YP\AJ
Sample : 02045-01 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
WC1-1-20230322

Integration File: autoint1.e
Quant Time: Mar 24 02:11:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.049	236217	2.347 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032323\
Data File : FG011647.D
Signal(s) : FID1A.ch
Acq On : 23 Mar 2023 19:37
Operator : YP\AJ
Sample : 02045-01 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
WC1-1-20230322

Integration File: autoint1.e
Quant Time: Mar 24 02:11:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG031523.M
Quant Title :
QLast Update : Wed Mar 15 18:43:49 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

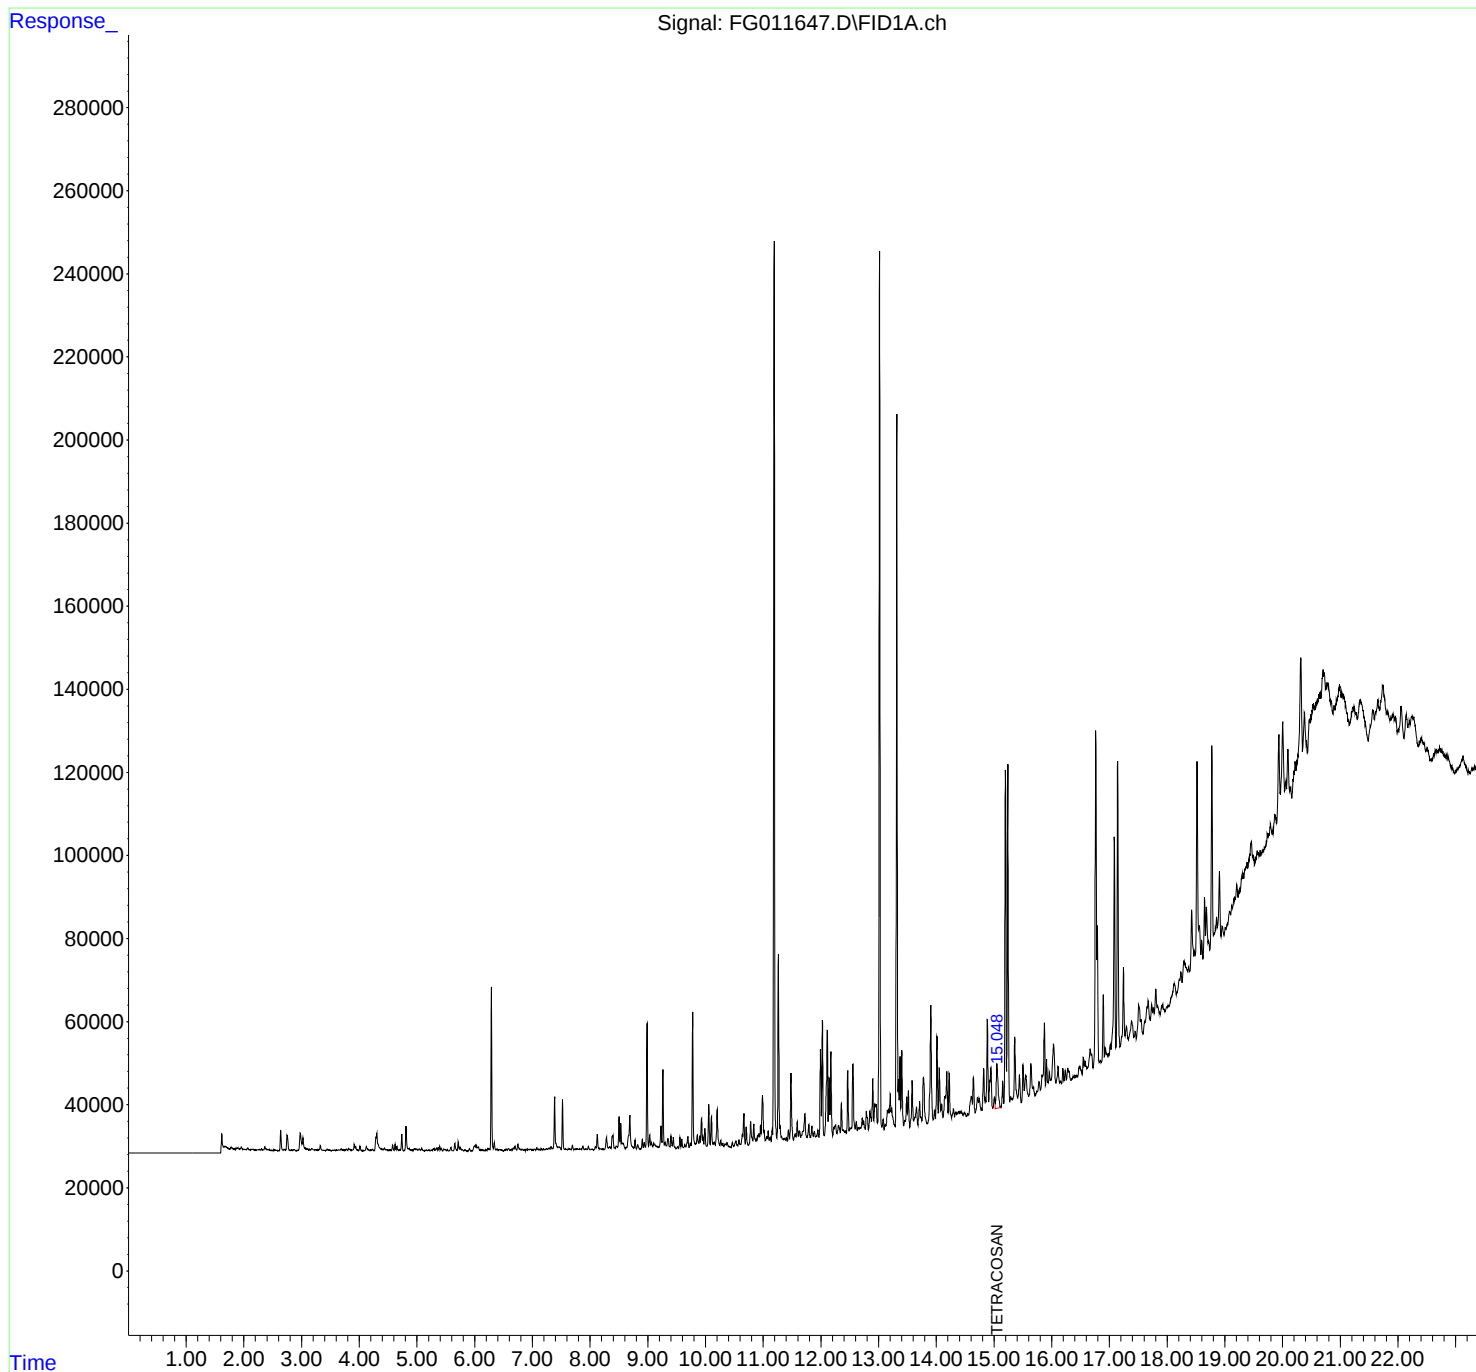

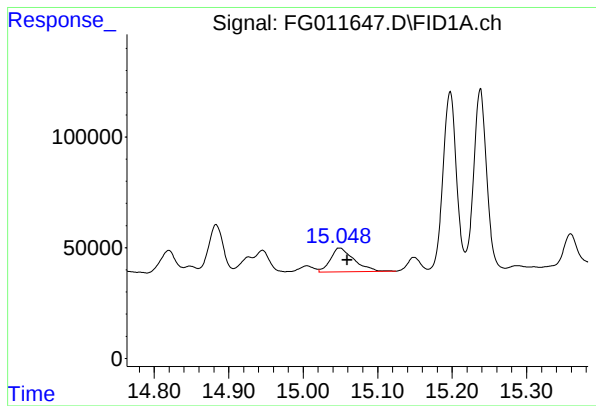

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.049 min
Delta R.T.: -0.010 min
Response: 236217
Conc: 2.35 ug/ml

Instrument :
FID_G
ClientSampleId :
WC1-1-20230322