

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032622\
 Data File : FG009414.D
 Signal(s) : FID1A.ch
 Acq On : 26 Mar 2022 10:34
 Operator : AJ\MA
 Sample : N2094-01 100X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 26 23:04:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032522.M
 Quant Title :
 QLast Update : Sat Mar 26 00:33:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
7) N-EICOSANE	12.558	74688	0.478 ug/ml
10) N-TETRACOSANE	14.778	55525	0.360 ug/ml
13) N-TRIACONTANE	17.699	66907	0.469 ug/ml
14) N-DOTRIACONTANE	18.527	90498	0.681 ug/ml
15) N-TETRATRIACONTANE	19.317	37381	0.320 ug/ml
16) N-HEXATRIACONTANE	19.980f	92092	0.934 ug/ml
17) N-OCTATRIACONTANE	20.749	369581	4.263 ug/ml
18) N-TETRACONTANE	21.628f	79450	0.935 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032622\
Data File : FG009414.D
Signal(s) : FID1A.ch
Acq On : 26 Mar 2022 10:34
Operator : AJ\MA
Sample : N2094-01 100X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 26 23:04:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032522.M
Quant Title :
QLast Update : Sat Mar 26 00:33:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

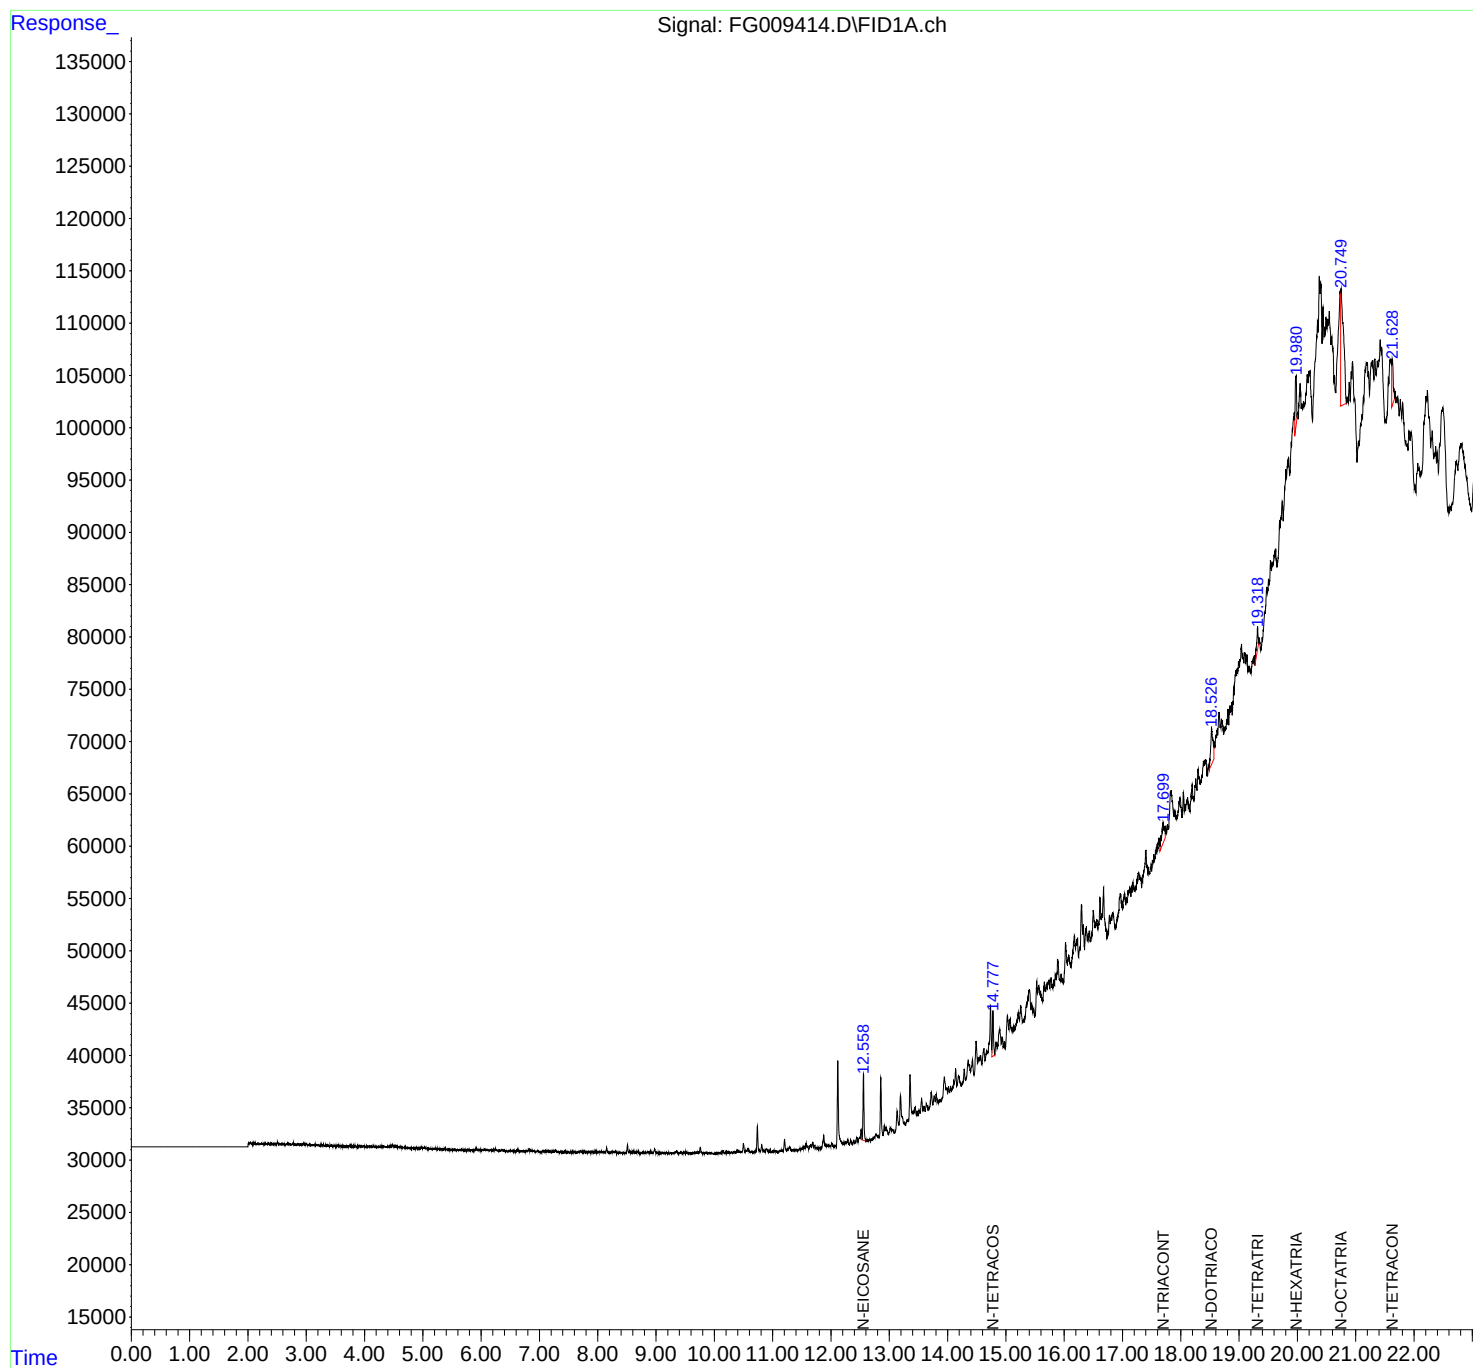


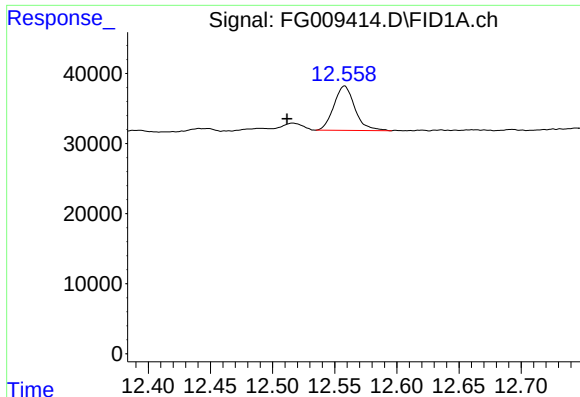

#7 N-EICOSANE


R.T.: 12.558 min
Delta R.T.: 0.046 min
Response: 74688
Conc: 0.48 ug/ml

Instrument :
FID_G
ClientSampleId :

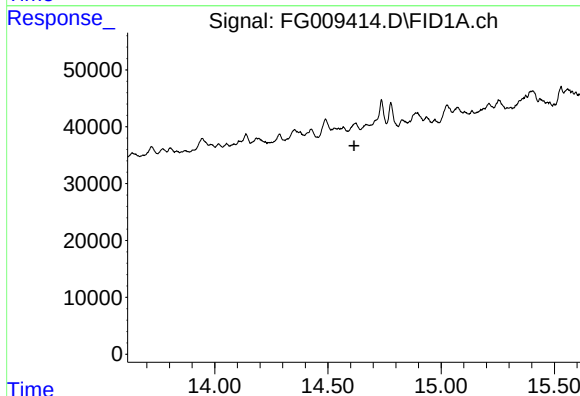


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.615 min
Response: 0
Conc: N.D.

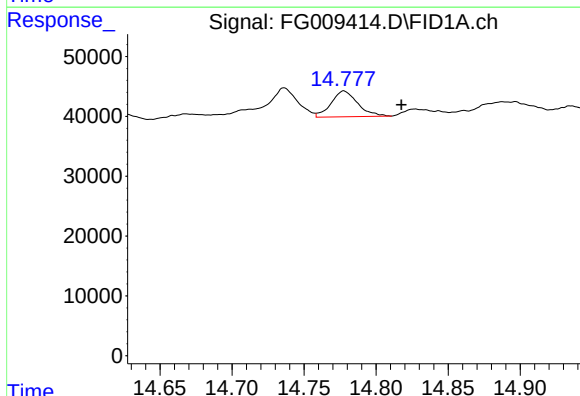


#10 N-TETRACOSANE

R.T.: 14.778 min
Delta R.T.: -0.040 min
Response: 55525
Conc: 0.36 ug/ml

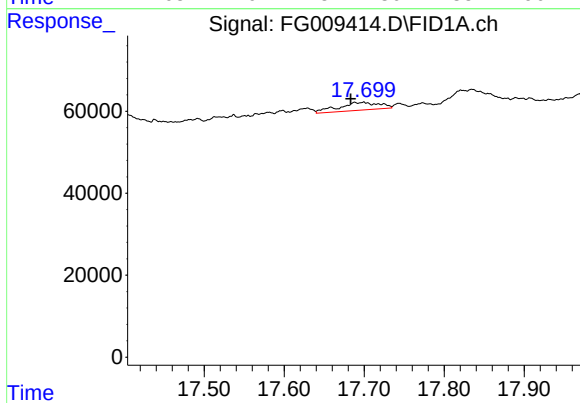

#13 N-TRIACONTANE


R.T.: 17.699 min
Delta R.T.: 0.016 min
Response: 66907
Conc: 0.47 ug/ml

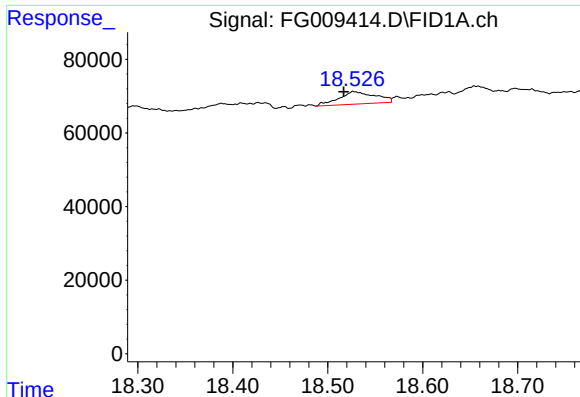

#14 N-DOTRIACONTANE


R.T.: 18.527 min
Delta R.T.: 0.010 min
Response: 90498
Conc: 0.68 ug/ml

Instrument :
FID_G
ClientSampleId :

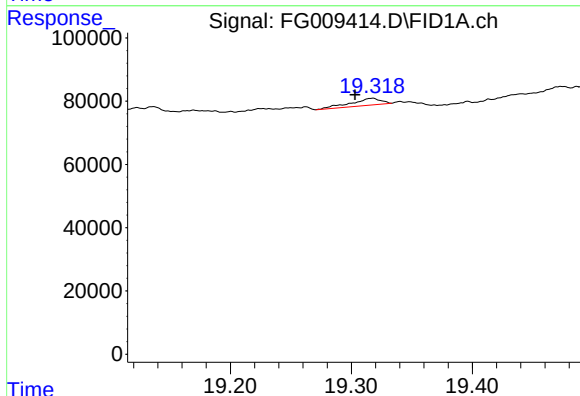


#15 N-TETRATRIACONTANE

R.T.: 19.317 min
Delta R.T.: 0.014 min
Response: 37381
Conc: 0.32 ug/ml

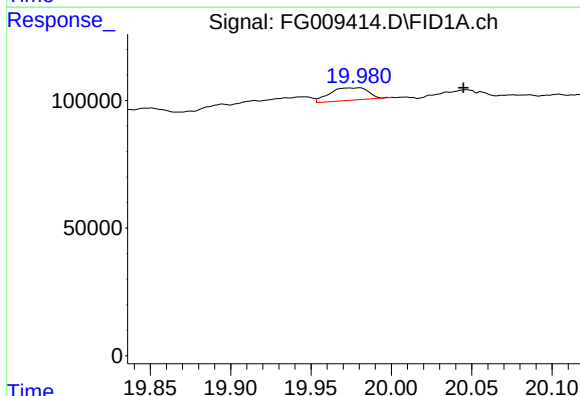


#16 N-HEXATRIACONTANE

R.T.: 19.980 min
Delta R.T.: -0.065 min
Response: 92092
Conc: 0.93 ug/ml

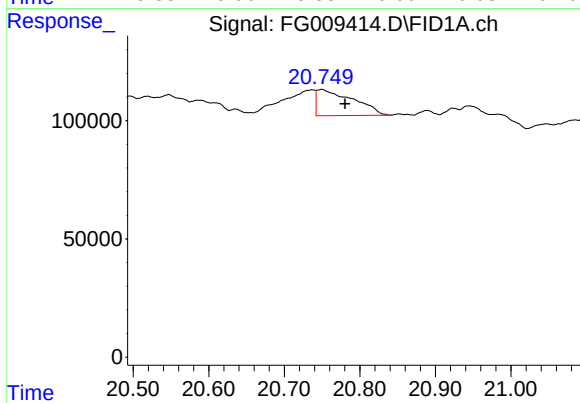

#17 N-OCTATRIACONTANE

R.T.: 20.749 min
Delta R.T.: -0.031 min
Response: 369581
Conc: 4.26 ug/ml

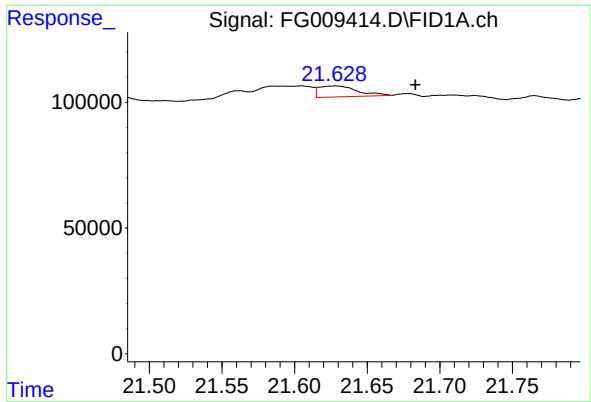

#18 N-TETRACONTANE

R.T.: 21.628 min
Delta R.T.: -0.055 min
Response: 79450
Conc: 0.93 ug/ml

Instrument :
FID_G
ClientSampleId :