

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032622\
Data File : FG009424.D
Signal(s) : FID1A.ch
Acq On : 26 Mar 2022 16:06
Operator : AJ\MA
Sample : PB143591BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 26 22:46:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032522.M
Quant Title :
QLast Update : Sat Mar 26 00:33:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.628	2090988	15.173 ug/ml
Target Compounds				
15)	N-TETRATRIACONTANE	19.324	46359	0.397 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG032622\
Data File : FG009424.D
Signal(s) : FID1A.ch
Acq On : 26 Mar 2022 16:06
Operator : AJ\MA
Sample : PB143591BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 26 22:46:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032522.M
Quant Title :
QLast Update : Sat Mar 26 00:33:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

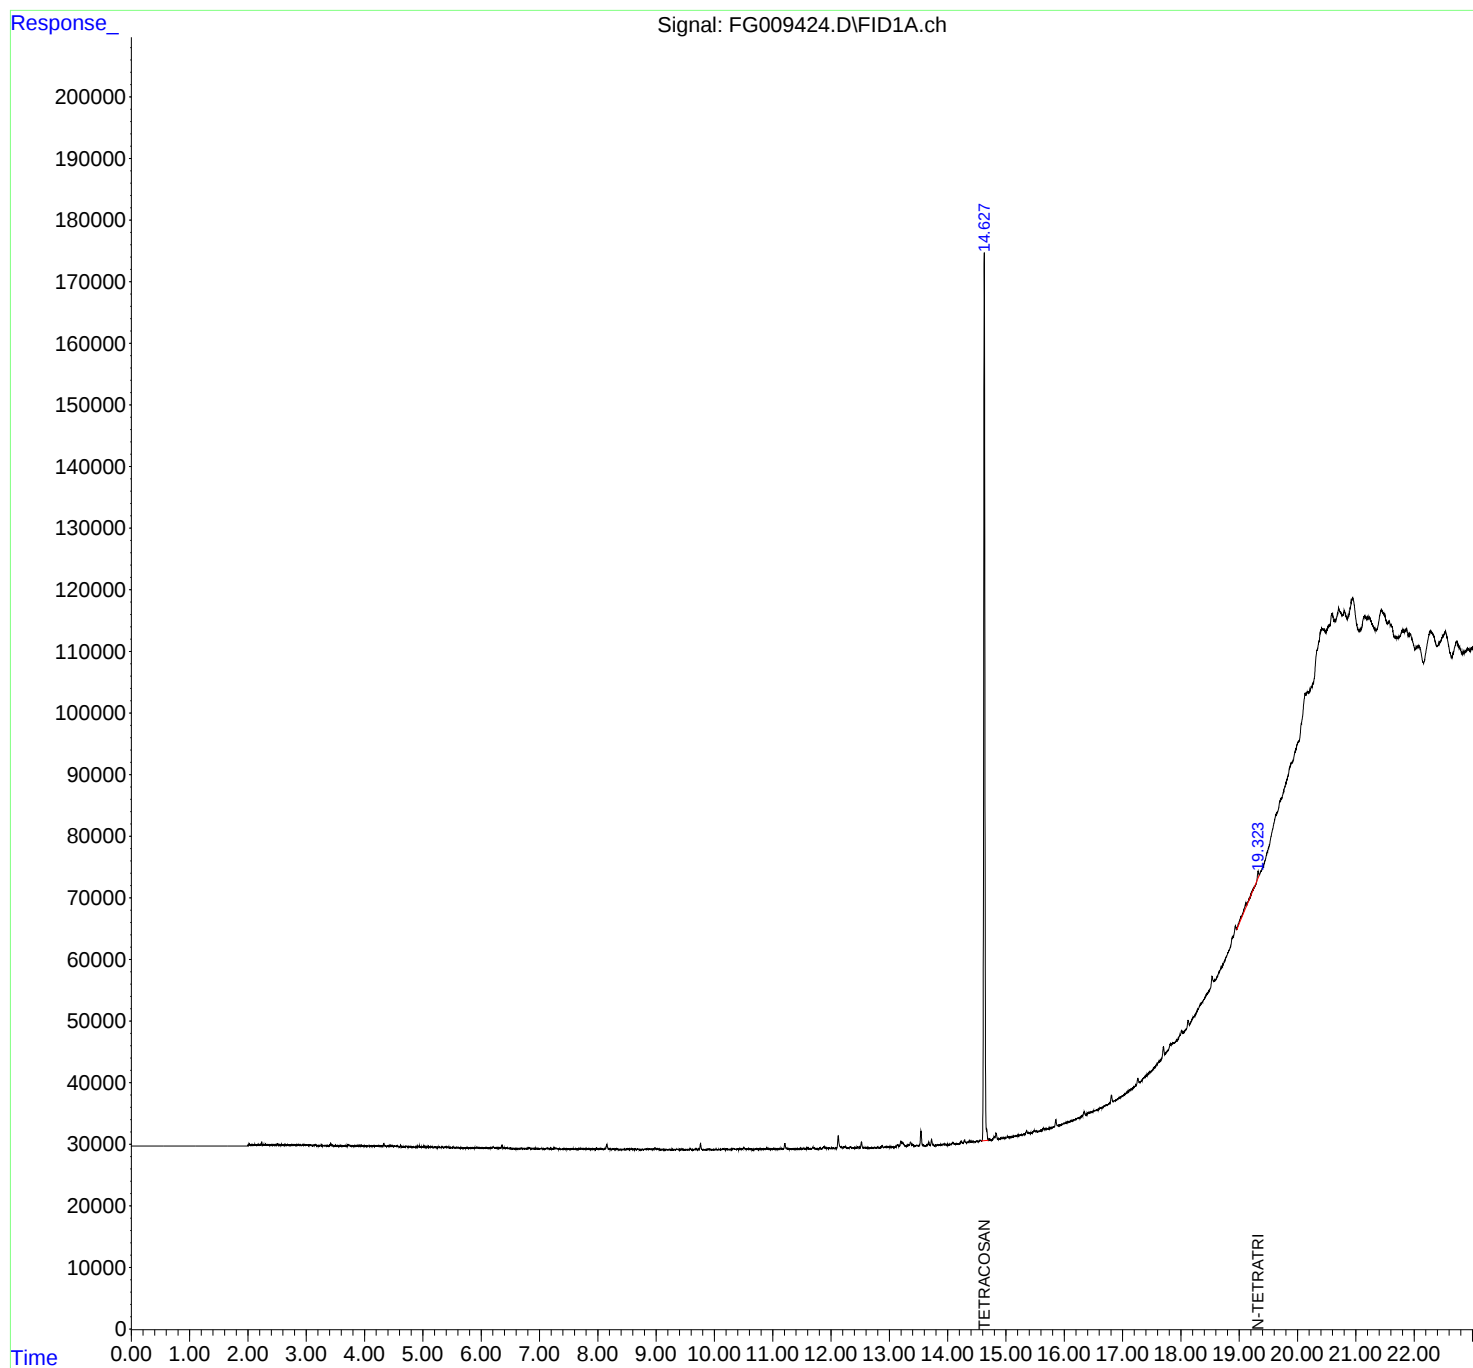


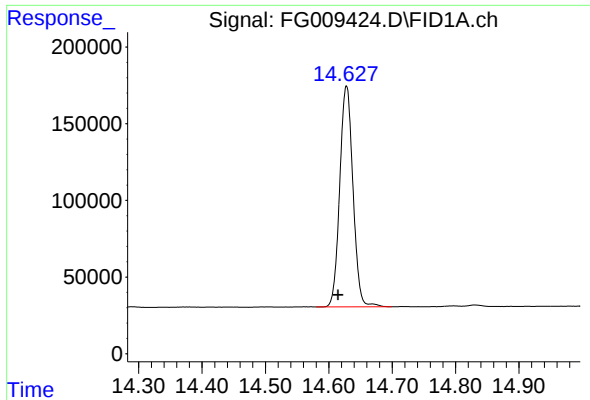

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.628 min
Delta R.T.: 0.013 min
Response: 2090988
Conc: 15.17 ug/ml

Instrument :
FID_G
ClientSampleId :

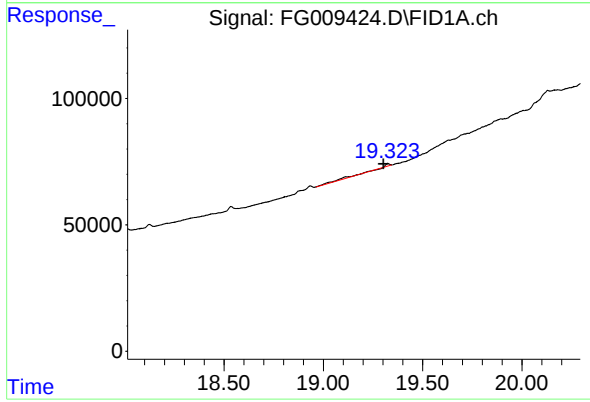

#15 N-TETRATRIACONTANE

R.T.: 19.324 min
Delta R.T.: 0.021 min
Response: 46359
Conc: 0.40 ug/ml